

A survey on wireless body area networks for eHealthcare systems in residential environments

Article

Accepted Version

Ghamari, A., Janko, B., Sherratt, S. ORCID: <https://orcid.org/0000-0001-7899-4445>, Harwin, W. ORCID: <https://orcid.org/0000-0002-3928-3381>, Piechockic, R. and Soltanpur, C. (2016) A survey on wireless body area networks for eHealthcare systems in residential environments. *Sensors*, 16 (6). 831. ISSN 1424-8220 doi: <https://doi.org/10.3390/s16060831> Available at <https://centaur.reading.ac.uk/65749/>

It is advisable to refer to the publisher's version if you intend to cite from the work. See [Guidance on citing](#).

Published version at: <http://www.mdpi.com/1424-8220/16/6/831>

To link to this article DOI: <http://dx.doi.org/10.3390/s16060831>

Publisher: MDPI

All outputs in CentAUR are protected by Intellectual Property Rights law, including copyright law. Copyright and IPR is retained by the creators or other copyright holders. Terms and conditions for use of this material are defined in the [End User Agreement](#).

www.reading.ac.uk/centaur

CentAUR

Central Archive at the University of Reading

Reading's research outputs online

1 *Type of the Paper (Review)*

2 **A Survey on Wireless Body Area Networks for** 3 **eHealthcare Systems in Residential Environments**

4 **Mohammad Ghamari** ^{1,*}, **Balazs Janko** ², **R. Simon Sherratt** ², **William Harwin** ², **Robert**
5 **Piechockic** ³, **Cinna Soltanpur** ⁴

6 ¹ Department of Electrical and Computer Engineering, University of Texas at El Paso, El Paso, Texas, USA

7 ² School of systems engineering, University of Reading, Reading, UK

8 ³ School of Electrical and Electronic Engineering, Bristol University, Bristol, UK

9 ⁴ Department of Electrical and Computer Engineering, University of Oklahoma, Norman, Oklahoma, USA

10 * Correspondence: mghamari@utep.edu; Tel.: +1-915-383-4996

11 Academic Editor: name

12 Received: date; Accepted: date; Published: date

13 **Abstract:** The progress in wearable and implanted health monitoring technologies has strong
14 potential to alter the future of healthcare services by enabling ubiquitous monitoring of patients. A
15 typical health monitoring system consists of a network of wearable or implanted sensors that
16 constantly monitor physiological parameters. Collected data are relayed using existing wireless
17 communication protocols to the base station for additional processing. This article provides
18 researchers with information to compare the existing low-power communication technologies that
19 can potentially support the rapid development and deployment of WBAN systems, and mainly
20 focuses on remote monitoring of elderly or chronically ill patients in residential environments.

21 **Keywords:** Biomedical; eHealthcare; Information and Communications Technology (ICT);
22 Telemonitoring; Wireless Body Area Network (WBAN); Wireless Technology.

24 **1. Introduction**

25 The ageing population around the world has been rapidly growing as a result of increased longevity,
26 mainly attributable to the substantial improvement in nourishment, medicine and public health. In
27 the United Kingdom alone, the population over the age of 85 is predicted to nearly triple by 2035 [1];
28 in the United States, the population over the age of 65 is estimated to double by 2040 [2]; in the
29 People's Republic of China, the population over the age of 60 is expected to double by 2040 [3]; and
30 Japan will have the eldest population in human history by the year 2050 with an average age of 52
31 years [4].

32 Simultaneously, public-funded healthcare systems in many developed countries are currently
33 confronting an increase in the number of people diagnosed with chronic diseases such as obesity and
34 diabetes. These chronic illnesses are not simply a result of ageing population but are due to
35 inappropriate diet, sedentary lifestyle and insufficient physical activity. As reported by the World
36 Health Organization (WHO), diabetes is estimated to become the seventh leading cause of death in
37 2030 [5]. Due to its chronic nature, diabetes is an expensive illness not only for individual patients
38 but also for healthcare systems as well.

39 These estimates and statistics indicate the fact that, continuously providing healthcare services to
40 patients who are diagnosed with chronic conditions and increasing number of elderly people with
41 various health difficulties is significantly increasing the cost of healthcare systems. Therefore,
42 healthcare systems are becoming unsustainable in their current form. According to scientists, early
43 disease detection and diagnosis is extremely important; on the one hand, it assists to effectively slow

44 the progress of illness; on the other hand, it helps to significantly reduce the cost of healthcare
45 systems.

46 It is, however, possible to utilize the latest technological advances in WBAN systems along with ICTs
47 for the early detection and prevention of potential diseases that may occur later in the people's lives.
48 This can be done by integrating ultra-low-power non-invasive and/or invasive sensor nodes into
49 WBAN systems for continuous monitoring of health conditions. Each node within a WBAN system
50 is capable of capturing physiological data such as Electrocardiogram (ECG), Electroencephalography
51 (EEG), respiratory rate, body temperature and movement and transmits the collected data either as
52 raw samples or low-level post-processed information to a base station wirelessly in order to be further
53 analyzed and processed. A WBAN system is able to provide long-term health monitoring of people
54 without limiting their daily activities. Such a system can be utilized to develop an intelligent and
55 inexpensive healthcare monitoring solution which can be used as part of a diagnostic process. The
56 future system will be able to remotely monitor elderly people and chronically ill patients in their own
57 residential environments where they are most relaxed and comfortable, and to minimize expensive
58 hospitalization costs and reduce frequent hospital visits.

59 There are similar published studies in this area such as [6] and [7] that investigate some aspects of
60 WBAN research such as physical and data link layer, and also compare a number of low-power radio
61 technologies. The primary contribution of this paper is not only to investigate and compare the
62 existing low-power on-body communication technologies, but also to consider the requirements and
63 challenges of these low-power wearable technologies to communicate with the home infrastructure.
64 Therefore, this paper considers the applicability and practical use of the existing low-power wearable
65 technologies in a residential environment.

66 The rest of this paper is organized into five sections. Section 2 presents an overview of a typical
67 eHealthcare project that is being carried out by a number of institutions and summarizes some of the
68 important requirements and design considerations of wireless communication technologies that can
69 potentially be used in WBAN systems. Section 3 reviews a number of existing low-power
70 communication technologies that are appropriate candidates for remote health monitoring
71 applications. Section 4 compares and discusses the advantage and disadvantage of using the existing
72 low-power technologies. Section 5 discusses the future prospects of remote health monitoring
73 systems. Section 6 provides a brief overview of some of the most recent research articles published in
74 the area of telemonitoring systems and finally Section 7 provides a conclusion to this article.


75 **2. Sensor Platform for Healthcare**

76 A unique approach to developing a new type of sensor platform for residential eHealthcare is being
77 carried out by the Universities of Bristol, Reading and Southampton. The aim of this project (termed
78 SPHERE) [8] is not to design and fabricate a new generation of sensors but rather to take advantage
79 of recent advances in WBAN systems along with ICTs to continuously monitor chronically ill patients
80 along with elderly people in their own residential environment. The new sensor platform is intended
81 to be multipurpose, inexpensive and scalable; it will be simple to use which make it appropriate for
82 all people especially those with a range of chronic diseases and the elderly. The ultimate sensor
83 platform will be capable of providing a more independent life style for vulnerable people with health
84 conditions inside their own residence where they are most comfortable. Long-term monitoring of
85 people's health is managed by a system where human intervention is not required. The eHealthcare
86 system is linked via the internet to a remote server where physicians or back-end algorithms are able
87 to check the health status of patients. The proposed sensor platform will offer health monitoring and
88 medical supervision to a wide range of chronic diseases that can be upgraded regularly. The SPHERE
89 project utilizes the latest advancements in ultra-low power sensor technologies, which has resulted
90 in miniaturized different types of body sensors in order to be able to obtain required physiological
91 information from monitored residents. The physiological data is usually collected by one or multiple

92 body sensor nodes within a wireless network. The collected database contains important and
 93 sometimes vital information of monitored people, such as different types of activities, health status
 94 and etc. The system also consists of an intelligent Decision-Making Unit (DMU), in which, an
 95 appropriate decision will be made based on analyzed data. For instance, in case of emergency,
 96 warning messages will be sent to medical providers or family members.

97 2.1. Residential Environment eHealthcare System Architecture

98 A typical architecture of a residential environment eHealthcare system consists of four layers as
 99 shown in Figure 1. Each layer of this architecture is further explained in more detail as follows. The
 100 BAN layer (layer 1) incorporates a number of sensor nodes operating within a wireless network.
 101 Sensor nodes in this layer are designed such that they can be placed on the human body as very small
 102 patches (on-body sensors), sewed into fabric (wearable sensors), or implanted under the skin (in-
 103 body sensors).

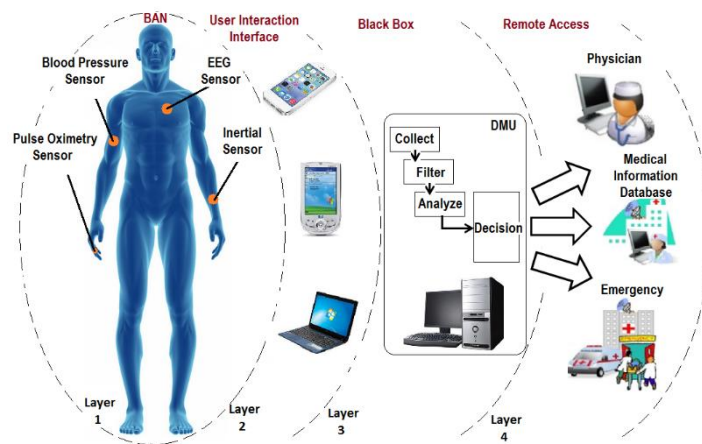

104 **Figure 1.** This is Four-layer typical architecture of eHealthcare system.

105 Such sensors continuously capture and relay vital parameters. However, depending on the
 106 functionalities and computation capabilities of nodes, data may require low-level on-tag processing
 107 prior to transmission. The collected data then may either initially be relayed to a central coordinator
 108 on the body or may be transmitted directly to the upper layers for further processing. The required
 109 transmission power by a sensor node in an off-body communication is mainly dependent on a
 110 number of factors such as Body Path Loss (BPL), Receive Noise Figure (RNF) and Signal to Noise
 111 Ratio (SNR) [9]. BPL determines the amount of the power absorbed by the human body during data
 112 transmission and is highly dependent on the selected operating frequency. Generally, lower
 113 operating frequencies have lower Specific Absorption Rate (SAR), whereas SAR at higher frequencies
 114 increases. RNF is also a device-dependent factor. Each device has its own RNF and is indicated in its
 115 datasheet. SNR however is influenced by the quality of the overall communication link. The
 116 performance of SNR can be improved by a number of techniques such as Error Control Coding (ECC)
 117 techniques and Single-Input and Multiple-Output (SIMO) methods [10] [11].

118 Layer 2 contains user interaction devices. Depending on the selected wireless communication
 119 protocol, different devices may be required to be used. For instance, Bluetooth-based sensor nodes
 120 require Bluetooth-based monitoring devices such as smartphones or PDAs. Layer 2 acts as an Access
 121 Point (AP). APs are usually located within a room environment. Each room is equipped with an AP,
 122 where wireless devices are connected to a wired network, Wi-Fi or other relevant standards.
 123 Collected data from this layer is required to be transferred to an upper layer (layer 3) in order to be
 124 prepared for the final destination. From room (layer 2) to black box (layer 3), there are a number of
 125 home networking possibilities that need to be considered.

126 There are three ‘room-to-box’ scenarios which are explained in more detail as follows. First scenario
 127 provides an approach based on dedicated cabling. In this scenario, either both data and power are
 128 transferred over a cable (e.g. Power over Ethernet (POE)) or data and power are transferred over
 129 separate cables (e.g. power over mains and data over Ethernet). The main disadvantage of this
 130 scenario is the requirement for cable installation which adds repetition complexity and cost to the
 131 system. Table 1, lists some of the existing wired home networking technologies that can potentially
 132 be used to transfer the data over the cables.

133

Table 1. Possible wired home networking technologies.

Characteristic	RS-485	CAN	Ethernet
Network Topology	Bus	Bus	Star
Theoretical Max Bandwidth	35 Mbit/s	1 Mbit/s	10 Mbit/s
Practical Bandwidth	1 Mbit/s	1 Mbit/s	2 Mbit/s
Stack Size (Heavy on Resources)	Light	Light+	Heavy
Management of Cabling	Complicated	Complicated	Straight Forward

134 The second scenario relies on Power Line Communication (PLC) technology, where data and power
 135 are transferred over mains. The main advantage of this scenario is the use of existing electrical wiring
 136 infrastructure and electrical outlets. PLC is a reliable technology and in terms of cost, it is less
 137 expensive than a dedicated cabling scenario. However, embedded based standards for PLC are
 138 limited in bandwidth. Another important disadvantage of PLC technology is that data may be lost
 139 due to an unexpected power outage.

140 The final scenario is based on existing wireless communication protocols such as Wi-Fi or ZigBee in
 141 order to transfer the collected data from rooms to black box. The biggest advantage of this method of
 142 data transfer is that no cable installation is required. However, this communication method is less
 143 reliable when compared to dedicated cabling and PLC technology.

144 The third layer of the proposed system architecture as depicted in Figure 1 consists of a the DMU as
 145 an automatic computing system which performs all major computing operations and is connected to
 146 the Internet. It is the main core of the solution where all important decisions are made. The role of
 147 DMU is to collect, filter and analyze the information. The aim of the DMU is to create a typical
 148 example of resident’s environment that includes a comprehensive database of resident’s medical
 149 profile. The DMU is able to recognize resident’s conditions based on the information obtained from
 150 a number of sensors which are transformed into knowledge and a list of user-defined policy rules.
 151 Subsequently, appropriate decisions are made automatically regarding the health status of
 152 inhabitant. The DMU is connected to a back-end medical institution such as a hospital in which
 153 physicians are able to consider people’s health status.

154 The last layer (layer 4) of this architecture as shown in Figure 1 provides healthcare services to
 155 patients. The analyzed data stored in the DMU is delivered to a remote server in a hospital, where
 156 medical practitioners have access to it. In this layer, two different types of services may be provided
 157 by healthcare personnel: healthcare services and emergency services.

158 2.2. Taxonomy and Requirements

159 This section summarizes the primary requirements and design considerations of wireless
160 communication technologies that can potentially be applied in WBAN systems.

161 2.2.1. Low-Power Consumption

162 Low-power consumption is considered to be one of the most important and challenging requirements
163 in WBAN systems. Devices in WBAN systems mainly consume energy during sensing vital
164 information, wireless communication and data processing. However, compared to sensing
165 information and data computation, wireless communication consumes a significant amount of
166 energy. Thus, reducing the energy consumption of data transmission during communication can
167 conserve considerable amounts of the energy reserves. In almost all WBAN devices, batteries are the
168 main source of power supply, but they are also the largest component in terms of weight and volume
169 compared to other electronic components. Since WBAN devices are meant to be wearable, batteries
170 must be kept small and the energy usage of the devices are required to be minimized. This is
171 important because in many WBAN applications such as pacemakers, wearable devices must be able
172 to operate for very long duration of time without being recharged or replaced. In such applications
173 in particular, prolonging the useful lifetime is crucial. Many techniques have been proposed in the
174 past to lower the power consumption of such devices. As an example, an energy-efficient hybrid
175 system has recently been proposed by Ghamari et al. [12] to minimize the required transmission
176 energy consumption of such systems by utilizing energy harvesting techniques and low-power MAC
177 protocols. In order to minimize power consumption, it is also important that the upper layer, the
178 application layer, uses a better strategy of sampling and transmitting data that is more convenient
179 for its application. As an example, the system can reduce the sampling rate of pulse when the user is
180 at rest according to the motion sensor. Dieter et al. [13] and Krause et al. [14] showed how selective
181 sampling strategies can decrease the power consumption of such systems which results in an increase
182 in the deployment lifetime of wearable technologies. Furthermore, authors in [15] believe that, in
183 order to lower the power consumption, it is also possible to reduce the sampling rate below the
184 Nyquist rate while still achieving an acceptable quality reconstruction.

185 2.2.2. Transmission Reliability and Latency

186 Data transmission reliability and latency are two extremely important factors in patient monitoring
187 applications. High reliability and low latency of data transfer ensures that real time data is
188 successfully transmitted and is immediately accessible to healthcare providers. Reliability directly
189 influences the quality of patient monitoring. It can be life-saving in many situations and in a worst-
190 case event; it can be disastrous when a life threatening incident has not been observed or detected.

191 On-body channel modeling is another key consideration that has significant impact on the robustness
192 of the communication link. On-body radio propagation channels are mainly influenced by the
193 frequent body movements and dynamic characteristic of the communication channel. Although
194 complicated analysis techniques such as Finite-Difference Time-Domain (FDTD) is able to provide
195 an accurate representation of static on-body radio propagation as shown in [16], extending such
196 analysis into dynamic on-body channel modeling cases is typically too costly. As a result of that many
197 studies focus on statistical techniques or uncomplicated analytical approaches [17] [18].

198 In addition, data transmission reliability and latency are mostly relied on the design of Physical
199 (PHY) and Medium Access Control (MAC) layers. In order to achieve optimal reliability and network
200 efficiency, appropriate MAC layer protocols are required to be designed to fulfill the particular needs
201 of specific applications [10] [11]. Reliability of WBAN systems can also be determined in terms of
202 their major Quality of Service (QoS) parameters such as transmission loss rate, delay profile and delay
203 jitter.

204 2.2.3. Data Rates

205 Due to the great diversity of the applications in WBAN systems, data rates differ greatly ranging from
206 low data rate sensors focused mainly on on-body monitoring at few kbps to high data rate systems
207 designed for multimedia data streams of several Mbps [19]. Information may also be transmitted in
208 bursts, though this way of transmitting information is not considered energy efficient due to the fact
209 that burst transmission sends out very high data transmission rate with very short transmission
210 durations. In medical applications, the reliability of the WBAN systems also depends on the
211 employed data rates as low data rate devices are able to manage high BER environments, whereas,
212 devices with higher data rates are most suitable to be used in lower BER conditions [20].

213 2.2.4. Security and Privacy

214 The transmission of health-related information between on-body sensors and monitoring devices in
215 WBAN systems and subsequently over the internet to central controllers in hospitals is strictly private
216 and confidential. Health-related information must be encrypted so that the patient's privacy is
217 protected. Healthcare professionals who have access to information must be confident that the
218 patient's vital information is not tampered with or altered and did truly originate from the monitored
219 individual. Furthermore, an overly secure system might disallow healthcare professionals from
220 accessing vital health-related information in certain emergency events and thus jeopardize patient's
221 life. Moreover, enriching the current systems with security and privacy mechanisms significantly
222 increases the cost of energy for communication which results in more power drain from small
223 batteries [19].

224 3. Candidate Wireless Technologies

225 This section reviews the latest wireless communication technologies that are able to support the rapid
226 development and deployment of BAN systems.

227 3.1. Popular Low-Power Wireless Technologies

228 3.1.1. Bluetooth Low Energy (BLE)

229 As part of the Bluetooth 4.0 standard, an alternative to classic Bluetooth was introduced known as
230 Bluetooth Low Energy (BLE) [21]. BLE was initially developed by Nokia in 2006. It was designed to
231 provide an extremely low power idle mode, uncomplicated device discovery and highly reliable
232 transfer of data. BLE is able to wirelessly connect miniature, low-power devices to mobile terminals
233 which make it an appropriate candidate for the health-monitoring (BAN) applications. BLE is
234 hardware-optimized version of Bluetooth because of its main differences such as data packet format,
235 radio transceiver and baseband digital signal processing compared to classic Bluetooth. BLE is able
236 to provide up to 1 Mbps data rate. Since BLE utilizes fewer numbers of channels for pairing BLE
237 devices, it consumes considerably less time (few milliseconds) for device discovery and
238 synchronization compared to seconds for Bluetooth. This is significantly valuable for resource-
239 limited and latency-critical devices such as those used in health-monitoring applications. BLE
240 employs a simplified protocol stack and is mainly concerned on short-range, star-topology network
241 with uncomplicated routing algorithms.

242 3.1.2. IEEE 802.15.4 and ZigBee

243 IEEE 802.15.4 [14] and ZigBee [23] are two widely used radio standards in BAN applications. IEEE
244 802.15.4 technology includes physical (PHY) and Medium Access Control (MAC) layer protocols
245 focusing on low data rate and medium-range wireless communications which makes it an
246 appropriate solution for health-monitoring applications.

247 Similar to IEEE 802.15.4, ZigBee is an enhanced version which provides additional layer protocols
248 such as network, security and application layers that reside on top of physical and MAC layers

249 defined by IEEE 802.15.4. The main purpose of both standards is to provide low power solution for
250 battery-powered devices. The physical layer utilizes Direct Sequence Spread Spectrum (DSSS)
251 modulation technique for interference mitigation and the MAC layer also utilizes Carrier Sense
252 Multiple Access with Collision Avoidance (CSMA/CA) for channel access. The ZigBee standard
253 provides support for flexible network topology. Devices in a ZigBee network are distinct between
254 Reduced Function Device (RFD) and Full Function Device (FFD). FFDs are able to set up a mesh
255 network where low duty cycle reduced function devices join the network as leaf nodes. In addition,
256 ZigBee fully supports the low duty cycle operation of nodes (sensor nodes turn off their radios most
257 of the time to reduce energy expenditure).

258 Contrary to ZigBee, classic Bluetooth does not support low duty cycling operation. In Bluetooth
259 devices, a slave node must be kept synchronized to the master node for data transmission. As a result
260 of that, there is an increase in 'radio on' period which in turn leads to increased energy consumption.
261 The ZigBee Alliance incorporates several public profiles which simplifies distribution of systems with
262 interoperable multi-supplier ZigBee-based devices. For instance, ZigBee has recently developed a
263 profile termed Personal Health and Hospital Care (PHHC) [24]. The aim of this profile is to provide
264 reliable and secure monitoring of non-invasive, non-critical healthcare applications mainly focused
265 on physical fitness, chronic disease and aging. The PHHC profile also fully supports ISO/IEEE 11073
266 standard [25] and utilizes the ISO/IEEE 11073 protocol for exchange of medical information.

267 Moreover, the ZigBee Alliance has recently introduced an optional feature in the ZigBee 2012
268 specification. This feature is termed ZigBee PRO Green Power [26]. Green Power provides adequate
269 power for battery-less devices with harvested energy and allows them to actively join ZigBee PRO
270 2012 networks.

271 Furthermore, IEEE 802 has recently introduced the first international WBAN standard called IEEE
272 802.15.6 [27]. The main purpose of this standard is to provide a short-range, low-power and extremely
273 reliable communications in the vicinity of or inside the human body. IEEE 802.15.6 is targeted to serve
274 a range of medical and non-medical applications.

275 3.2. Alternative Low-Power Wireless Technologies

276 3.2.1. Classic Bluetooth

277 Classic Bluetooth is a Wireless Personal Area Network (WPAN) technology [28] where a number of
278 Bluetooth devices (up to eight) form a short-range personal network known as piconet. In Bluetooth,
279 slave devices must be paired and synchronized with a master device before data communication
280 starts. This is usually achieved via the use of common clock between the communicating devices.
281 Bluetooth operates in the 2.4 GHz ISM frequency band; it utilizes frequency hopping mechanism
282 among 79 channels with an average rate of 1,600 hops per second to minimize interference. The
283 Bluetooth standard classifies devices into three groups based on transmission power and
284 corresponding coverage area. The wireless communication range supported by the standard
285 provides adequate coverage for WBAN communications. The Bluetooth SIG has developed the
286 Health Device Profile (HDP) [29] capable of providing usage models for fitness and healthcare
287 devices. HDP is also able to wirelessly connect devices such as glucose meters, pulse oximeters,
288 weight scales, thermometers and blood pressure monitors to sink devices such as cell phones, PDAs,
289 laptops and personal computers.

290 3.2.2. ANT

291 ANT [30] is a low-power proprietary wireless technology designed and developed for a broad range
292 of wireless sensor network (WSN) applications. ANT is specifically appropriate for low data rate
293 battery powered sensor nodes and covers a range of network topologies from simple peer-to-peer to

294 complex mesh networks. ANT is a candidate for wireless connectivity in battery powered
295 applications such as health monitoring where ultra-low power consumption is required. ANT
296 operates in the 2.4 GHz frequency band, supports a data rate of 1Mb/s and employs TDMA scheme
297 to address interference issues. ANT+ facilitates wireless communication of devices from different
298 companies by providing predefined network parameters and data payload structures including
299 device profiles. Existing ANT+ device profiles consist of heart rate monitors, stride-based speed and
300 distance monitors, bike speed and power. Several upcoming device profiles include weight scales,
301 multi-sport speed and distance, and environment sensors.

302 3.2.3. RuBee

303 RuBee [31] is considered an alternative to Radio-Frequency Identification (RFID). It is a bidirectional
304 active wireless protocol that employs long wave magnetic signals (not RF signals) to transmit and
305 receive 128 byte packets of data within a local network. RuBee is based on the IEEE 1902.1 [32]
306 standard and is specifically designed to provide high security in harsh environments. Similar to the
307 IEEE 802 standards, RuBee enables the networking of devices by employing point-to-point active
308 radiating transceivers. This protocol operates at the low frequency end, 131 kHz. Similar to WiFi,
309 Bluetooth and ZigBee, RuBee is an on-demand packet based protocol but with lower data rate. In
310 addition, RuBee's low operating frequency provides a significant benefit in terms of power
311 consumption. It can provide a battery life of up to fifteen years using a single lithium button cell
312 battery with a distance range of 1 to 50 feet. However, RuBee's low operating frequency requires a
313 bigger antenna size which makes this technology a likely inappropriate candidate for BAN
314 applications where the size of antenna plays an important role. In contrast to RFID, RuBee does not
315 have signal reflections and cannot be blocked by materials such as steel and liquid. Therefore, it is a
316 robust technology especially in harsh environment visibility and security applications [33] [34].

317 3.2.4. Sensium

318 Sensium [35] is an ultra-low power wireless platform mainly designed to provide customized health
319 services for chronic disease management applications [36]. Sensium is capable of providing an ultra-
320 low power monitoring of vital health signs such as PH levels, blood glucose and ECG signals. The
321 main aim of Sensium is to be embedded in a digital plaster to be prescribed by physicians. Sensium
322 operates in the 900 MHz frequency band and supports a data rate of 160 kb/s. Sensium is considered
323 as one of the leading ultra-low power wireless technologies for low data-rate on-body applications.
324 Sensium utilizes a master/slave communication structure, in which an on-body slave node transmits
325 multiple vital signs to a personal server such as smart phone, PDA or a personal computer from time
326 to time. Since sensium utilizes a star topology, joining a network is managed centrally. Energy
327 consumption of nodes is also managed centrally; nodes are programmed to keep their radios in sleep
328 mode until they are given time slots by central server.

329 3.2.5. Zarlink

330 Zarlink [37] [38] is a proprietary ultra-low power RF transceiver specifically designed for medical
331 implantable applications. Zarlink utilizes Cyclic Redundancy Check (CRC) error detection along with
332 Reed-Solomon error correction scheme to provide a highly reliable communication link. It operates
333 in the MICS (402-405 MHz) and ISM (433-434 MHz) bands. Zarlink supports data rates of up to 800
334 kb/s. Zarlink is able to operate in both an implant and a base station. Depending on the selected
335 system type, different requirement is needed especially in terms of power consumption. Therefore,
336 Zarlink has specified two important operation modes: Implantable Medical Device (IMD) mode and
337 base mode. When Zarlink is configured as an IMD mode, the radio is asleep most of the time which
338 consumes only μ W of power compared to mW of power in other modes. However, communication
339 between two nodes cannot occur if either node's radio is in sleep mode. Therefore, a mechanism is
340 required to wake up the receiver's radio to ensure the sender's transmit and receiver's listen

341 operations coincide. This can be done by either utilizing an ultra-low power 2.4 GHz radio or directly
342 by using the IMD processor. Zarlink is considered as one of the leading ultra-low power wireless
343 technology for low-data rate medical implantable applications (TRX = 5 mA, low-power mode = 1
344 mA and ultra-low power wakeup circuit = 250 nA).

345 3.2.6. Z-Wave

346 Z-Wave [41] is a proprietary wireless communication protocol mainly designed for automation in
347 home and light commercial environments. Z-Wave was initially developed by ZenSys (it is now a
348 division of Sigma Designs) [42] and is currently managed by the Z-Wave Alliance [43]. One of the
349 main advantages of Z-Wave compared to some other technologies is that it operates in the sub-1 GHz
350 band (around 900 MHz) which avoids interference with other wireless technologies operating in the
351 crowded 2.4 GHz band such as WiFi, Bluetooth and ZigBee. Z-Wave technology utilizes a number of
352 low-cost low-power RF transceiver chips which are embedded into home electronic devices such as
353 lighting, intercom and entertainment systems. Z-Wave uses a low-power wireless technology to
354 communicate with Z-Wave-based devices. This technology is optimized to provide reliable
355 transmission of small data packets from a control unit to Z-Wave devices in a network. Z-Wave
356 protocol utilizes frame check sequence, frame acknowledgement, retransmission, CSMA/CA and
357 complex routing algorithms to ensure reliable communication in multipath environment of a
358 residential house. Z-Wave supports mesh networking, provides 9.6 kb/s and 40 kb/s data rates, and
359 uses Gaussian Frequency-Shift Keying (GFSK) modulation scheme. Z-Wave recently introduced the
360 Z-Wave 500 series, a next generation upgrade to the Z-Wave chip and module which supports a
361 higher data rate of up to 100 kb/s. Z-Wave is able to include up to 232 nodes in a Z-Wave network.
362 This technology defines two different types of devices: controllers and slaves. Controllers have
363 unidirectional control over slave devices. They are responsible for sending commands to slave
364 devices, which receive the task and send back the corresponding answer [44].

365 3.2.7. Insteon

366 Insteon [39] is a proprietary mesh networking technology specifically designed for home and
367 personal electronics applications. Insteon makes use of both Radio Frequency (RF) signals and
368 home's existing electrical wiring infrastructure (PLC) to transmit data from one device to another.
369 Insteon is able to utilize RF-only devices, power-line-only devices or can simultaneously support both
370 types of communication systems. Therefore, it is considered as one of the most reliable home
371 automation technology. Insteon devices are called peers because all Insteon devices are able to
372 transmit, receive and relay other messages completely independent of a controller. Insteon
373 communication range can be extended by means of a multi-hop approach. In this method, an Insteon
374 network uses two or more hops to deliver information from a source to a destination. Similar to Z-
375 Wave, Insteon also limited the maximum number of hops allowed for each message to four. In
376 addition, in PLC applications, Insteon operates at 131.65 kHz and uses Binary Phase-Shift Keying
377 (BPSK) modulation technique; in RF applications it operates in the ISM (902-924 MHz) band and uses
378 Frequency-Shift Keying (FSK) modulation scheme. Insteon utilizes Automatic Repeat request (ARQ)
379 scheme to achieve reliable data transmission over unreliable or noisy communication channels.
380 Insteon supports instantaneous data rates of 13.165 kb/sec. It also supports a number of encryption
381 methods such as rolling-code, managed-key and public-key [40].

382 3.2.8. Wavenis

383 Wavenis is a wireless protocol architecture created as a proprietary technology by Coronis systems
384 and promoted by the Wavenis Open Standard Alliance [45]. Wavenis is specifically designed to
385 provide an ultra-low power and long-range wireless solution for a vast range of Machine to Machine
386 (M2M) applications such as industrial process control, environmental monitoring and healthcare
387 monitoring. In the majority of M2M applications, devices are expected to have low data rates and to

388 operate on battery. However, recharging or replacing batteries not an easy task in many situations,
389 saving battery power without compromising reliability is an important challenge. Moreover, a high
390 link budget is needed to achieve adequately long-range communication in a number of M2M
391 applications. Wavenis is an appropriate candidate to provide solution for these challenges. The main
392 features of Wavenis technology include power conservation, reliability, network coexistence and
393 resistance against interference. Wavenis operates worldwide in the 433 MHz, 868 MHz and 915 MHz
394 ISM bands. It supports different data rates of 4.8 kb/s, 19.2 kb/s and 100 kb/s, uses GFSK modulation
395 scheme and employs fast Frequency-Hopping Spread Spectrum (FHSS) technology. The MAC layer
396 of the Wavenis protocol consists of two transmission techniques: synchronous and asynchronous. In
397 the synchronous communication networking mode nodes are equipped with a combination of CSMA
398 and TDMA channel access schemes. In this case, a randomly computed time slot is allocated to a node
399 willing to acquire the channel. Prior to transmission in the allocated time slot, the node listen to the
400 shared medium to check for any on-going transmission. If the shared medium is occupied by other
401 nodes, the node calculates a new time slot for its next transmission. However, asynchronous
402 communication networking applies in applications where reliability plays an important role such as
403 security systems and in such applications CSMA/CA mechanism is used [44].

404 3.2.9. BodyLAN

405 BodyLAN is an ultra-low power, low-cost and reliable BAN platform created as a proprietary
406 technology by FitLinxx [46]. BodyLAN is designed to be used in a vast variety of applications such
407 as consumer electronics, activity and wellness devices, medical devices and fitness equipment. In
408 terms of power usage, BodyLAN provides much lower power consumption rate compared to
409 Bluetooth devices. This wireless technology uses a single radio channel, short burst duration and
410 extremely low duty cycle. BodyLAN utilizes GFSK modulation technique which prevents BodyLAN
411 packets from colliding with 802.11g/ Orthogonal Frequency-Division Multiplexing (OFDM)/ DSSS
412 packets. BodyLAN operates in the 2.4 GHz ISM band and supports data rates of 250 kb/s and 1 Mb/s.
413 It also utilizes a peer-to-peer network topology without centralized timing. Devices in a BodyLAN
414 network are categorized into two groups of transmit-only and transmit/receive devices. In terms of
415 security, BodyLAN encrypts frame payloads and dynamically changes algorithms based on device
416 addresses and timing plans. In addition, following the collection of data, the ActiHealth network
417 utilizes a secure VPN connection between the ActiHealth data server and application servers in order
418 to guarantee the security of the collected information.

419 3.2.10. Dash7

420 Dash7 [47] is a proprietary open source, ultra-low power and long-range wireless communication
421 protocol which was initially designed for military usage and has been adapted for use in commercial
422 applications. Dash7 technology is based on the ISO/IEC 18000-7 open standard using an active RFID.
423 This technology is currently managed by the Dash7 Alliance which offers interoperability among
424 Dash7-based devices. Dash7 operates in the 433 MHz band, supports nominal and maximum data
425 rates of 28 kb/s and 200 kb/s respectively. The main features of Dash7 includes very long
426 communication range of up to 2 km, ultra long battery life, AES support and low latency for
427 connecting with moving objects. Dash7 networks are specifically suited for low power consumption
428 applications where data transmission is sporadic and operated considerably slower such as telemetry
429 systems. Dash7 utilizes Bursty, Light, Asynchronous, Stealth, and Transitive (BLAST), i.e. Dash7
430 networking technology is especially appropriate to be used in bursty and light (packet sizes are
431 maximized to 256 bytes) applications with asynchronous communication. In addition, Dash7-based
432 devices are inherently portable and upload-centric, thus, the devices are not required to be managed
433 by fixed infrastructure such as base stations. Dash7-based devices are being used today in a vast
434 number of applications such as building automation, smart meters, hazardous material monitoring,
435 manufacturing and warehouse optimization, inventory management and mobile payments.

436 3.2.11. ONE-NET

437 ONE-NET [48] is a proprietary open source standard, mainly designed to solve the problems of a
438 wireless network in the home environment. ONE-NET is specifically optimized to support low-
439 power long-range applications. One of the main characteristics of ONE-NET is that it is open to most
440 proprietary software and hardware and is capable of being implemented with a vast range of low-
441 cost low-power off-the-shelf microcontrollers and transceivers from numerous manufacturers such
442 as Texas Instruments, Silicon Labs and Freescale. ONE-NET operates in different frequency ranges
443 of 433 MHz, 868 MHz, 915 MHz and 2400 MHz. It uses Wideband FSK modulation technique and
444 supports base and maximum data rates of 38.4 kb/s and 230 kb/s respectively. ONE-NET takes
445 advantage of different network topologies for connecting ONE-NET-based devices. It utilizes peer-
446 to-peer (P2P), star and multi-hop topologies with the master node organizing the P2P connections.
447 Star topology is able to minimize cost and complexity of peripherals. Multi-hop network topology
448 utilizes two or multiple wireless hops in order to cover larger communication area. ONE-NET is able
449 to support maximum indoor and outdoor communication ranges of 100 m and 500 m respectively.
450 ONE-NET wireless technology is specifically optimized for low-power consumption such as battery-
451 operated devices. According to ONE-NET specification, low-duty-cycle battery-operated ONE-NET-
452 based devices are able to achieve up to five years battery life on an AA or AAA Alkaline battery. In
453 terms of security, ONE-NET utilizes the extended tiny encryption algorithm version two with thirty-
454 two iterations [40].

455 3.2.12. EnOcean

456 EnOcean [49] is a proprietary energy harvesting wireless sensor technology designed to be applied
457 in a vast variety of applications such as building automation and control systems, transportation,
458 cold-chain management, environmental monitoring and health monitoring. EnOcean is promoted by
459 EnOcean Alliance to ensure interoperability of EnOcean products among different device vendors.
460 EnOcean wireless technology is specifically optimized to provide solutions for ultra-low power
461 consumption and energy harvesting applications. EnOcean-based devices utilize ultra-low power
462 electronics and micro energy converters to enable wireless communications among battery-free
463 sensors, switches, controllers and gateways. The main purpose of EnOcean's energy harvesting
464 technology is to derive energy from surroundings such as light, motion, pressure and transform them
465 into electrical energy that can be utilized. Recently, EnOcean is ratified as a new international wireless
466 standard by the International Electrotechnical Commission (IEC) as ISO/IEC 14543-3-10 to accelerate
467 the development of energy-optimized wireless sensor networks. Products based on EnOcean are
468 designed to operate without batteries and are engineered to run maintenance-free. EnOcean operates
469 in frequency ranges of 315 MHz, 868.3 MHz and 902 MHz. It uses Amplitude-Shift Keying (ASK)
470 modulation technique, utilizes relatively small data packets (limited to 14 bytes) and supports data
471 rates up to 125 kb/s. This technology is also able to support maximum indoor and outdoor
472 communication ranges of 30 m and 300 m respectively.

473 3.2.13. Emerging Intra-Body Communication Technologies

474 Intra-Body Communication (IBC) technology is one of the emerging possible solutions for providing
475 an ultra-low power communication over very short range links that specifically target WBAN
476 applications. This technology is a non-RF wireless communication that utilizes human body as the
477 medium for data transmission. IBC has recently been outlined in the newly ratified IEEE 802.15.6
478 standard and has shown to have advantages in terms of energy efficiency over many existing low-
479 power RF protocols as it is able to transmit data with ultra-low transmission power below 1 mW [50]
480 [51].


481 The IBC technology utilizes three main approaches to wirelessly interconnect in-body implanted
482 devices: ultrasonic communication, capacitive coupling and galvanic coupling techniques. Ultrasonic

483 communication has recently been proposed in [52] to address the limitations of RF propagation in
 484 the human body. In water-based environments such as the human body where 65 percent is
 485 composed of water, radio waves are not perfectly suited. This is mainly due to the fact that water
 486 typically absorbs some portion of the radio waves. Thus, more amount of energy is required to
 487 successfully transfer the RF signal in the human body. Hence, acoustic waves are considered one of
 488 the possible transmission technologies of choice for in-body communications as they are recognized
 489 to propagate better than RF signals in media mostly composed of water.

490 In the capacitive coupling technique, human body is capacitively coupled to the surrounding
 491 environment [50]. In this technique, a current loop through the external ground creates the signal
 492 between the body channel transceiver. Alternatively, galvanic coupling method is performed by
 493 coupling Alternating Current (AC) in to the human body. In this technique, AC current is flowed
 494 through the body and human body is considered as a waveguide [50] [51].

495 The energy efficiency advantage of these two coupling techniques over wireless protocols is mainly
 496 due to two reasons. One is due to the existence of lower path loss which does not include the
 497 otherwise detrimental effects of body shadowing in RF communications. The other reason is due to
 498 the utilization of wearable electrodes that are used as communication interface rather than low-
 499 impedance antennas. Moreover, in terms of security, IBC technology was shown itself to be more
 500 secure and less susceptible to interference compared to RF communication which makes it a possible
 501 low-power communication solution for Body Area Network (BAN) applications.

502 Nevertheless, IBC technology cannot solely be used in BAN systems. The data gathered by IBC-based
 503 sensors are required to be transmitted to a base station for further processing. For this reason, IBC
 504 technology must be combined with one of the existing energy efficient communication protocols such
 505 as ZigBee or Bluetooth Low Energy (BLE) [53]. Figure 2 shows a typical architecture of a possible
 506 energy efficient BAN system. In this scenario, IBC technology is employed for intra-body
 507 communications. IBC based sensor devices transfer the health-relevant information through the body
 508 to a central node which acts as a coordinator. This central coordinator is in charge of establishing a
 509 communication link between on-body devices and a base station. Thus, it uses one of the existing
 510 low-power communication protocols to transfer the collected data to a base station.

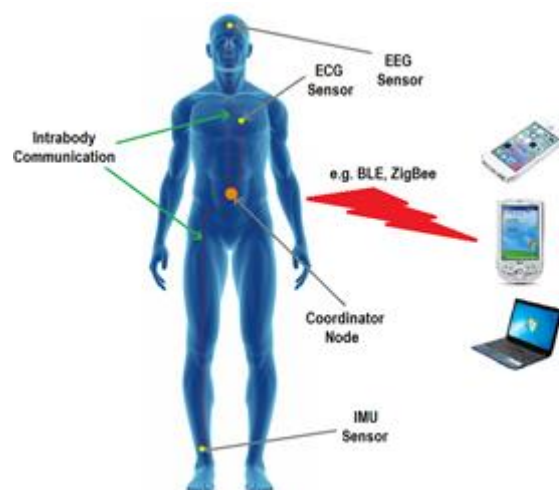

511 **Figure 2.** Intra-body communications combined with existing low-power protocols.

512 4. Discussion

513 In wearable health monitoring systems, energy efficient functioning of wearable devices is highly
514 dependent on the selection of appropriate communication protocols. This is because wireless
515 communication, unlike sensing and computation, consumes a significant amount of energy in the
516 sensor nodes. Thus, a suitable selection of low-power communication technology can substantially
517 increase the useful lifetime. This section highlights some of the important features of possible low-
518 power communication technologies that must be taken into account when choosing a particular
519 technology choice.

520 There are a number of low-power wireless communication protocols that can accomplish this task.
521 Out of these protocols, ZigBee and Bluetooth are most broadly used. The preference of Zigbee over
522 Bluetooth/BLE or vice versa can be made based on the following factors:

523 4.1. Protocol Efficiency

524 Protocol efficiency needs to be considered before selecting a low-power communication protocol. It
525 greatly influences the energy efficiency of the selected protocol. This is because an inefficient
526 communication protocol spends the majority of its time transferring overhead information rather
527 than transmitting the actual payload data. Thus, little data may be transferred over a fixed duration
528 of time and devices transferring the information may quickly run out of power. The efficiency of
529 protocols can be calculated based on the ratio of actual payload information to the total length of the
530 data packets. It is therefore very easy to compute the protocol efficiency of ZigBee and BLE by
531 considering their packet formats (see Table 3); BLE has protocol efficiency of 66%, whereas ZigBee
532 has protocol efficiency of 76%.

533 Although, the results show that ZigBee is more protocol efficient than BLE, in many low data-rate
534 low-power health monitoring systems wearable sensor nodes are only required to partially utilize
535 the total available payload space to transfer data, hence, lower protocol efficiency does not necessarily
536 mean that a particular protocol is inappropriate.

537 4.2. User Flexibility

538 According to the Bluetooth Special Interest Group (SIG), the majority of the Bluetooth-based
539 smartphones will support BLE by 2018. This will offer great flexibility to end users, as a BLE-enabled
540 smartphone can potentially be utilized as an access point. ZigBee needs a ZigBee-enabled device as
541 an access point (currently there are no mobile phones with ZigBee capabilities).

542 4.3. Communication Range

543 ZigBee is considered to be a wireless Local Area Network (LAN) technology, thus it covers a greater
544 range, whereas BLE is a wireless Personal Area Network (PAN) protocol and its range is more
545 limited. In a typical health monitoring system, there are scenarios in which collected data is required
546 to be transferred to an access point within a room distance. In these scenarios, both BLE and ZigBee
547 are considered as suitable protocols. However, in scenarios where data needs to be transmitted to a
548 local station located in the other side of the house, if no other home networking infrastructures such
549 as WiFi, PLC or Ethernet is employed, ZigBee is regarded as the better solution, simply because BLE
550 is unable to cover the required distance by itself.

551 4.4. Energy Efficiency

552 Without a proper, in-depth analysis of these protocols, very little can be derived in terms of their
553 energy efficiency. However, comparing the characteristics of these protocols can provide an
554 approximate estimation of their energy expenditures during data transmission. Multiple access
555 schemes are one of the important features that need to be considered more carefully as these can
556 affect the energy efficiency of protocols. BLE uses Frequency Division Multiple Access (FDMA) along

557 with Time Division Multiple Access (TDMA) schemes, whereas ZigBee employs CSMA/CA scheme.
 558 FDMA/TDMA schemes are more suitable to be used on high-load networks as they share the
 559 communication channel more efficiently and fairly, but are inefficient at low-load networks as there
 560 is usually delay in channel access. While the CSMA/CA scheme is more appropriate to be employed
 561 at low-load networks as there is no delay in channel access, is inefficient at high-load networks as
 562 packet collisions may happen. For more comprehensive comparison of ZigBee and BLE, see Tables
 563 2-5.

564

Table 2. Physical layer comparison of ZigBee and Ble

Characteristic	ZIGBEE	Bluetooth Low Energy
Frequency Band	2400, 868, 915 MHz	2400 MHz
Bit Rate	20 Kb/s (868 MHz), 40 Kb/s (915 MHz), 250 Kb/s (2400 MHz)	1 Mb/s
Modulation Type	BPSK, O-QPSK	GFSK
Spread Spectrum	DSSS	FHSS
Technology		
Nominal TX Power	-32 dBm to 0 dBm	-20 dBm to 10 dBm
Receiver Sensitivity	-85 dBm	-70 dBm
Number of Physical Channels	27 channels: 16 channels in the 2450 MHz, 10 channels in the 915 MHz, 1 channel in the 868 MHz	40 channels in FDMA: 3 advertising channels, 37 data channels
Channel Bandwidth	2 MHz (5 MHz wasteful spectrum)	2 MHz (no wasteful spectrum)

565

Table 3. Link layer comparison of ZigBee and Ble

Characteristic	ZIGBEE	Bluetooth Low Energy
Multiple Access Scheme	CSMA-CA, slotted CSMA-CA	FDMA, TDMA
Maximum Packet Size	133 Bytes	47 Bytes
Protocol Efficiency (ratio of payload to total packet length)	102/133 = 0.76 (76 Percent Efficient)	31/47 = 0.66 (66 Percent Efficient)
Error Control Method	ARQ,FEC	ARQ,FEC
CRC Length	2 Bytes	2 Bytes
Latency	< 16 ms (beacon-centric network)	< 3ms

Identifiers	16-bit short address	48-bit public device
	64-bit extended address	address 48-bit random device address

566

Table 4. Network layer comparison of ZigBee and Ble

Characteristic	ZIGBEE	Bluetooth Low Energy
Network Topology	P2P, Star, Cluster Tree, Mesh	P2P, Star
Single-hop / Multi-hop	Multi-hop	Single-hop
Nodes / Active Slaves	> 65000	Unlimited
Device Types	Coordinator, Router, End Device	Master, Slave
Networking Technology	PAN	PAN

567

Table 5. Comparison of other properties of ZigBee and Ble

Characteristic	ZIGBEE	Bluetooth Low Energy
Authentication	CBC-MAC	Shared Secret
Encryption	AES-CTR	AES-CCM
Range	100 Meters	10 Meters
Implementation Size	45 - 128 KB(ROM) 2.7 - 12 KB (RAM)	40 KB (ROM) 2.5 KB (RAM)

568 Alternative low-power wireless technologies include ANT, but also include recently developed
 569 proprietary technologies. These technologies usually are very constrained solutions that provide
 570 extremely low power requirements at the expense of much reduced data rate or range of
 571 communication. Some of them offer the flexibility of variable data rate and hence power
 572 consumption, and can operate at a number of radio frequencies.

573 A few of these protocols such as RuBee, Zarlink and Dash7 are only able to operate on lower
 574 frequency bands. Lower frequency bands are less crowded with radio services and they are less
 575 exposed to external interference, hence they have lower likelihood of packet collisions which results
 576 in lower power consumption. In addition, operating on lower frequency bands come with an
 577 advantage of good signal penetration through a variety of materials including the human body,
 578 however, the required antenna size is larger than those used at higher frequencies.

579 Among the low-power protocols, only ZigBee uses DSSS whereas BLE, Bluetooth and Wavenis
 580 employ FHSS. Spread spectrum techniques are employed for a range of reasons including increasing
 581 resistance to unwanted interference and noise. DSSS radios are believed to operate better for large
 582 data packets in low to medium interference environments, while FHSS radios operate better for small
 583 data packets in high interference environments. Moreover, FHSS radios perform better indoors and
 584 in harsh multipath environments because frequency hopping techniques are able to manage
 585 multipath fading environments by hopping to new frequency channels [54].

586 In terms of robustness, ANT, RuBee and Z-Wave only use error detection schemes such as CRC or
 587 Longitudinal Redundancy Check (LRC) whereas the rest of the protocols take advantage of an
 588 additional Forward Error Correction (FEC) technique along with error detection schemes. Error
 589 detection schemes are used in two-way communication systems in which packet retransmission will
 590 be requested by the receivers if errors are detected in the received data. This error control technique
 591 offers high transmission reliability and very low system complexity and is able to protect the
 592 information against most possible error occurrences over a comparatively quiet channel. However,
 593 applying a simple error-detection-only technique can also have a severe disadvantage. In erroneous
 594 channels, if the level of noise increases such that there is a high possibility that packets have at least
 595 one error, then the channel will quickly be occupied with retransmissions. As a consequence, no new
 596 information will be transmitted and the system throughput will decrease, and ultimately approach
 597 zero (This drawback affects many latency-sensitive applications such as health monitoring systems).
 598 Therefore, a combination of CRC and FEC techniques that most of the protocols use in this survey
 599 can protect the information in various channel conditions.

600 Many of these protocols such as BLE, Bluetooth, ANT, Z-Wave, Wavenis, BodyLAN and Dash7 use
 601 GFSK modulation while a number of other protocols such as Zarlink, Insteon and ONE-NET employ
 602 FSK modulation. GFSK modulation is an improved version of the FSK in which the data must be
 603 filtered via a Gaussian filter prior to modulating the carrier. This leads to a narrower power spectrum
 604 of the modulated signal which results in higher transfer speed of data in the same channel bandwidth
 605 [55]. In addition, GFSK modulation has the potential to cover a greater communication range
 606 compared to FSK modulation [56].

607 All of the protocols are equipped with at least one type of encryption or level of security. Some of
 608 these encryptions are strong while others are very limited and offer little protection. In addition,
 609 Bluetooth, RuBee, Dash7 and EnOcean provide alternative security engines within the same chip
 610 which may be beneficial in particular applications. Some applications require less stringent security,
 611 whilst others may be able to exploit the optional extra encryption methods at different times. It is
 612 difficult to mention which security technique is more appropriate as it is so application and
 613 regulatory dependent. However, the fact that all radios offer some method of securing the
 614 communication channel ensures a level of security.

615 Alternative radios may also provide benefits such as a flexible packet format (length) that may result
 616 in more efficient packing of data per transmission.

617 Most of these radios such as ZigBee, Wavenis and Dash7 do not require additional infrastructure in
 618 order to fully cover a residential area; however, some of them such as BLE, Bluetooth, Sensium and
 619 Zarlink may require more infrastructure to support a greater range. For more comprehensive
 620 comparison of alternative low-power wireless technologies, see Tables 6-13.

621 **Table 6.** Physical layer comparison of Bluetooth, Ant, RuBee, Sensium, Zarlink and Insteon

Characteristic	Bluetooth	ANT	RuBee	Sensium	Zarlink	Insteon
Frequency Band	2400 MHz	2400-2485 MHz	131 KHz	868 MHz, 915 MHz	402-405 MHz, 433-434 MHz	RF: 869.85, 915, 921 MHz Powerline: 131.5 KHz
Bit Rate	1-3 Mbps	1 Mbps	9.6 Kbps	50 Kbps	200/400/800 kbps	RF: 38.4 Kbps Powerline: 13.1 Kbps
Modulation Type	GFSK	GFSK	ASK, BPSK, BMC	BFSK	2FSK/4FSK	RF: FSK Powerline: BPSK
Spread Spectrum	FHSS	No	No	No	*	No

Technology						
Nominal TX Power	0/4/20 dBm	4 dBm	-20 dBm	-10 dBm	2 dBm	*
Receiver Sensitivity	-90 dBm	-86 dBm	*	-102 dBm	-90 dBm	-103 dBm
Number of Physical Channels	79	125	2	16	10 MICS, 2 ISM	*
Channel Bandwidth	1 MHz	1 MHz	*	200 KHz	*	*

622

623

Table 7. Link layer comparison of Bluetooth, Ant, RuBee, Sensusium, Zarlink and Insteon

Characteristic	Bluetooth	ANT	RuBee	Sensusium	Zarlink	Insteon
Multiple Access Scheme	TDMA	TDMA	*	TDMA, FDMA	*	TDMA + Simulcast
Maximum Packet Size	358 bytes	19 bytes	128 bytes	*	*	Standard: 10 bytes Extended: 24 bytes
Error Control Method	CRC, FEC	CRC	CRC	CRC, FEC	CRC, FEC	CRC, FEC
Checksum Length	1-byte/2-byte	2-byte	1-byte	*	*	1-byte
Identifiers	48-bit Public Device	*	32-bit	*	*	24-bit Module ID

624

Table 8. Network layer comparison of Bluetooth, Ant, RuBee, Sensusium, Zarlink and Insteon

Characteristic	Bluetooth	ANT	RuBee	Sensusium	Zarlink	Insteon
Network Topology	Piconet, Scatternet	P2P, Star, Tree, P2P Mesh		Star	P2P	Dual-mesh (RF & Powerline), P2P, Mesh
Single-hop/Multi-hop	Multi-hop	*	*	Single-hop	*	Multi-hop
Nodes/Active Slaves	8	65,000+1	Unlimited	8+1	*	Unlimited
Device Types	Master, Slave	Master, Slave	Controller, Responder	Master, Slave	*	All are peers
Networking Technology	PAN	PAN	PAN	PAN	PAN	PAN

625

Table 9. Comparison of other properties of Bluetooth, Ant, RuBee, Sensusium, Zarlink and Insteon

Characteristic	Bluetooth	ANT	RuBee	Sensusium	Zarlink	Insteon
Security	Optional Pre-Shared Key, 128-bit Encryption	AES-128 Data Encryption, Link Authentication	Optional AES Encryption, Private Key, Public Key	Public Key	*	Rolling Code, Public Key

Range	10 m	30 m On-Body Only	30 m	5 m On-Body Only	2 m In-Body Only	45 m(Outdoors)
Implementation Size	100 Kbytes (ROM), 30 Kbytes (RAM)	128 Kbytes (Flash)	0.5-2 Kbytes (SRAM)	48 Kbytes (RAM), 512 bytes (ROM)	*	3Kbytes (ROM), 256 Bytes (RAM)
Certification	Body	Bluetooth SIG	ANT+Alliance	None	None	Insteon Alliance
Proprietary	No	Yes	No	Yes	Yes	Yes

626

Table 10. Physical layer comparison of Z-Wave, Wavenis, BodyLan, Dash7, One-net and Enocean

Characteristic	Z-Wave	Wavenis	BodyLAN	Dash7	ONE-NET	EnOcean
Frequency Band	868, 908, 2400 MHz	433, 868, 915, 2400 MHz	2400 MHz	433 MHz	433, 868, 915, 2400 MHz	315, 868, 902 MHz
Bit Rate	9.6/40 Kbps, 200 Kbps	4.8/19.2/100 Kbps	250 Kbps, 1 Mbps	28, 55.5, 200 Kbps	38.4, 230 Kbps	125 Kbps
Modulation Type	GFSK	GFSK	GFSK	FSK, GFSK	Wideband FSK	ASK
Spread Spectrum	No	Fast FHSS	*	No	No	No
Technology						
Nominal TX Power	-3dBm	14 dBm (Max)	0 dBm	0 dBm	*	6 dBm
Receiver Sensitivity	-104 dBm	-110 dBm	-93 dBm	-102 dBm	*	-98 dBm
Number of Physical Channels	*	16 Channels @ 433 & 868 MHz, 50 Channels @ 915 MHz	1	8	25	*
Channel Bandwidth	*	50 KHz	*	216, 432, 648 KHz	*	280 KHz

627

628

Table 11. Link layer comparison of Z-Wave, Wavenis, BodyLan, Dash7, One-net and Enocean

Characteristic	Z-Wave	Wavenis	BodyLAN	Dash7	ONE-NET	EnOcean
Multiple Access Scheme	CSMA/CA	CSMA/TDMA, TDMA, CSMA/CA	CDMA	CSMA/CA	*	CSMA/CA
Maximum Packet Size	64 bytes	*	62 bytes	256 bytes	5 bytes	14 bytes
Error Control Method	LRC	FEC, Data Interleaving, Scrambling	CRC, FEC	CRC, FEC	*	CRC, FEC
Checksum Length	1-byte	No	*	2-byte	*	1-byte

Identifiers	32-bit (home ID), 8-bit (node ID)	48-bit MAC Address	*	EUI-64	*	*
-------------	--------------------------------------	--------------------	---	--------	---	---

629 **Table 12.** Network layer comparison of Z-Wave, Wavenis, BodyLan, Dash7, One-net and EnOcean

Characteristic	Z-Wave	Wavenis	BodyLAN	Dash7	ONE-NET	EnOcean
Network Topology	Mesh	P2P, Star, Tree, P2P, Ad-Hoc, Mesh, Repeater Star		BLAST, Mesh	P2P, Star, Mesh	P2P, Star, Mesh
Single-hop/Multi-hop	Multi-hop	Multi-hop	*	Multi-hop	Multi-hop	Multi-hop
Nodes/Active Slaves	232	Up to 100,000	*	2^32	4096	>4000
Device Types	Controller, Slave	Single Type	Single Type	Blinker, Endpoint, Gateway, Subcontroller	Master, Slave	Master, Slave
Networking Technology	PAN	LAN	PAN	PAN, LAN	PAN	PAN

630 **Table 13.** Comparison of other properties of Z-Wave, Wavenis, BodyLan, Dash7, One-net and EnOcean

Characteristic	Z-Wave	Wavenis	BodyLAN	Dash7	ONE_NET	EnOcean
Security	128-bit AES Encryption	128-bit AES Encryption	*	Private Key (i.e. XTEA2 AES 128), Public Key (i.e. Management ECC, RSA)	Algorithm, Key Management	Rolling Code, 128-bit AES Encryption, CMAC Algorithm, Private Key, Public Key
Range	30 m (Indoors), 100 (Outdoors)	200 m (Indoors), 1000 m (Outdoors)	122 m (Outdoors)	2000 m	100 m (Indoors), 500 m (Outdoors)	300 m (Outdoors), 30 m (Indoors)
Implementation Size	32-64 Kbytes (Flash), 2-16 Kbytes (SRAM)	48 Kbytes (Flash), 400 Bytes (RAM), 20 Bytes (Non-Volatile Memory)	*	8-16 KB (Built Size)	16 K (ROM), 1 K (RAM), 128 Bytes (Non-Volatile Memory)	32 KB (Flash), 2 KB (RAM)
Certification Body	Z-Wave Alliance	Wavenis Alliance	None	Dash7 Alliance	ONE-NET Allinace	EnOcean Allinace
Proprietary	Yes	No	Yes	No	No	No

631 Due to the limited range requirements of a residential environment eHealthcare system, full meshing
632 capability of any wireless communication platform may not be necessary, however if no meshing is
633 supported, the infrastructure must be extended so that the premises is fully covered. Alternatively,
634 multi-hop based routing of wireless communication packets may provide the required range of the
635 application, but this solution requires multiple nodes with adequate power budget.

636 Different protocols offer various connection management schemes. It may be considered a
637 disadvantage if a body-worn sensor node has to maintain link with specific infrastructure or other
638 sensor nodes. It may be advantageous if a link can be made and broken at any point without severely
639 affecting latency and power budget.

640 5. Future Prospects

641 Nowadays, smartphone devices are more pervasive, user-accepted and powerful than ever. A large
642 proportion of people carry their smartphones with them all the time and thus the idea of simple and
643 continuous connectivity is not inaccessible anymore [57]. Mobile health (termed as mHealth)
644 technologies have also experienced a slight change in direction from wearing and/or implanting body
645 sensors to carrying a powerful wireless device with multifunctional capabilities such as a smartphone
646 [58]. Healthcare providers may soon be able to monitor and measure vital signs without the need of
647 on-body and/or implanted sensors (non-contact vital sign monitoring) [59]. For example, researchers
648 from Rice University have been developing a non-contact video-camera system that can precisely
649 monitor and measure temperature, pulse and breathing rate from changes in a patient's skin color
650 [59]. Smartphones can also be independently used for sleep monitoring. For instance, iSleep [60] takes
651 advantage of the built-in microphone to detect the unconscious actions during sleep such as body
652 movement, coughing and snoring, which are closely associated with the perceived quality of sleep
653 people receive. Although, a more complete review of non-contact vital sign monitoring systems is
654 not in the scope of this article, a number of examples of such systems are described in the literature
655 [61-63]. The rest of this section is categorized into three parts. Part A summarizes a number of major
656 advantages of smartphone-based healthcare applications. Part B considers some challenges of such
657 solutions and finally part C explains the most areas of mHealth research that are expected to grow in
658 the near future.

659 5.1. Advantages of Smartphone-Based Healthcare Applications

660 A collection of different types of low-cost sensors (e.g. accelerometer, gyroscope, camera,
661 magnetometer, pedometer, goniometer, actometer, biometric and pressure) embedded in
662 smartphones have enabled these multifunctional devices to be applied in many aspects of future
663 healthcare systems. In addition, combination of some of these sensors such as biometric sensors with
664 big data has provided a potential for smartphones to hugely impact the future of healthcare systems.
665 For instance, people may habitually check their smartphones 100 times a day. This statistic
666 information can be used to enable smartphone devices to frequently obtain the user's facial scan. In
667 this way, vital signs such as heart rate or blood pressure can be measured [64]. If this technique is
668 used over a large population and such biometric data is collected in the cloud, contagious disease
669 outbreaks can be discovered more quickly [64].

670 With the prevalent use of smartphones and the appearance of fourth generation of mobile
671 telecommunications technology (4G) that provides higher speed mobile broadband internet access
672 services along with the ubiquity of Wi-Fi technology, healthcare informatics (an interdisciplinary
673 field combining healthcare, computer science and information science) is now able to overcome time
674 and location limitations. This is enormously important specifically in cases that an immediate
675 response is extremely critical or when a patient's condition is not stable and dynamically changing.

676 In contrast to intrusive wearable devices that impose a burden on user's daily activities, smartphones
677 are non-intrusive, non-obstructive and not required to follow a cumbersome usage protocol. This
678 results in reducing the possible usability complications.

679 Smartphones do not require supplementary hardware and many health-related mobile apps are
680 accessible and free which lead to a more cost-effective solution compared to traditional wearable
681 devices.

682 Smartphones have potential to manage chronic diseases such as Alzheimer's, Hypertension and
683 Diabetes. This can be done by frequent monitoring of patients through mobile apps or message
684 reminders regarding the drug dosage information.

685 5.2. Challenges of Smartphone-Based Healthcare Applications

686 There is an uncertainty regarding the usefulness of disease control by smartphones. Ryan et al. [65]
687 considered the cost-effectiveness of utilizing smartphone-supported self-monitoring of Asthma. He
688 discovered that self-management by smartphones were not cost-effective in patients. This means that
689 specific patient group will require careful, personalized treatment plan to address the specific needs
690 and problems of patients who are suffering from a particular disease [66].

691 While the use of smartphones present great opportunities to improve healthcare quality for patients
692 with chronic conditions, yet there has not been an effective strategy to move from pilot studies to
693 implementation in the wider population [67].

694 In addition, the care of the elderly possibly cannot simply rely on smartphones as elderly individuals
695 may be visually impaired, unable to use their hands effectively or even, unable to use the technology
696 at all.

697 5.3. Fastest Areas of mHealth Growth in the Near Future

698 Areas of mHealth that are expected to have the most growth potential in the near future are explained
699 as follows [68].

700 Patient monitoring is expected to have the fastest area of growth in the near future. This is because it
701 is capable to early detect and prevent potential diseases that may occur later in life. This also can help
702 to significantly reduce the cost of healthcare systems.

703 Patient location tracking is estimated to have the second most area of mHealth growth in the near
704 future. This is simply because the need to locate and track patients with chronic conditions such as
705 Alzheimer's and Dementia is great and thus the number of possible platforms proposing such
706 solutions are steadily increasing [68].

707 6. Summary of Recent Research Articles

708 One of the main goals of this paper is to provide a brief overview of the most recent technological
709 advances in the area of eHealthcare systems where healthcare providers are able to remotely monitor
710 patients through the state-of-the-art WBAN systems along with existing ICTs. Since this area of
711 research is able to significantly affect the existing healthcare systems by reducing the current
712 operational costs, it has attracted the attention of a large number of researchers and scientists during
713 the past decade and as a result of that many promising prototypes have been designed and
714 developed. This section attempts to consider some of the most recent scientific publications in the
715 field of telemonitoring systems for elderly and chronically ill patients.

716 In order to find the most relevant research articles, a number of scientific search engines such as the
 717 IEEE Xplore Digital Library, the ACM Digital Library and the PubMed database were searched. The
 718 survey is limited to recent articles no older than five years as the wireless technologies of concern
 719 were only adopted widely in this period. In order to select the related articles from a large number of
 720 papers appeared in the search results, the following specific inclusion criteria when examining the
 721 abstracts and main body of the texts were found, A) only articles consisting of on-body (including
 722 wearable) sensors that may or may not be considered along with off-body (ambient) sensors; B)
 723 articles that are more focused on elderly health monitoring and addressing chronic health issues; C)
 724 articles that use a type of wireless communication technology. In addition, this survey excluded
 725 scientific papers that mainly address in-body (implantable) sensors and ambient sensors (out of the
 726 scope of this survey). The research selected 35 articles out of the search results that are able to fulfill
 727 the selection criteria. The main information extracted from these 35 articles is presented in Table 14.

728 **Table 14.** Included published articles between 2010 and 2015

Publication	On-body OR Off-body Sensors	Monitoring Parameters	Wireless Comm & Gateway	Novelty
Mazilu, Blanke, Dorfman, Gazit, Mirelman, Hausdorff, Troster {2015} [69]	On-body	Body Positioning, Motion	Bluetooth, Smartphone	A wearable assistant for gait training for Parkinson Disease with Freezing of Gait
Taylor, Bernard, Pizey, Whittet, Davies, Hammond, Edge {2015} [70]	On-body	Body Positioning	Bluetooth, Smartphone	A wristband community alarm with in-built fall detector
Miranda, Calderon, Favela {2014} [71]	On-body	Spontaneous Blink Rate, Heart Rate	Bluetooth, Wi-Fi, PC	Anxiety detection technique using Google Glass
Kantoch, Augustyniak, Markiewicz, Prusak {2014} [72]	On-body	Skin Humidity, Heart Rate, Temperature, Body Positioning	Bluetooth, PC	Monitors ADL based on custom-designed wearable WSN
Papazoglou, Laskari, Fourlas {2014} [73]	On-body	Body Positioning, Motion	ZigBee, PC	A low-cost open architecture wearable WSN for healthcare applications
Ojetola, Gaura, Brusey {2015} [74]	On-body	Body Positioning	Bluetooth, PC	Presents a description of the dataset for simulation of falls, near-falls and ADL
Yan, Huo, Xu, Gidlund {2010} [75]	On-body Off-body	ECG, Pressure, Fire, Light, Moisture, Sound, Temperature	ZigBee, Laptop, PDA	A mixed positioning algorithm (object proximity positioning, signaling active positioning and signaling passive positioning)
Farre, Papadopoulos, Munaro, Rosso {2010} [76]	On-body Off-body	Heart Rate, Respiration, Inspiration & Expiration Time & Volume, Temperature & Humidity, Motion Activity & Fall Detection, Cough & Snoring Detection, Ambient Light, Carbon Monoxide,	Bluetooth, PDA	Addresses two specific diseases (Chronic Obstructive Pulmonary Disease and Chronic Kidney Disease)

		Volatile Organic Compound, Air Particle		
Vanveerdeghem, Torre, Stevens, Knockaert, Rogier {2014} [77]	On-body	Body Positioning	ZigBee, PC	Presents synchronous wearable WSN composed of autonomous textile nodes
Doukas, Maglogiannis {2011} [78]	On-body Off-body	Body Positioning, Audio Sound, Motion, Sound	ZigBee, PC	Audio data processing and sound directionality analysis in conjunction to motion information and subject's visual location is used to verify fall and indicate an emergency event
Lamprinakos, Kosmatos, Kaklamani, Venieris {2010} [79]	On-body Off-body	Heart Rate, Skin Temperature, Pulse Rate, Motion, Physical Contact	Bluetooth, WiFi, ZigBee, Z-Wave, GSM, IP, Home Base Station (with Hydra middleware)	Hydra Middleware is used to make it possible to achieve integration and self-organization of sensors
Cancela, Pastorino, Tzallas, Tsipouras, Rigas, Arredondo, Fotiadis {2014} [80]	On-body	Body Positioning, Motion	ZigBee, PC	A Parkinson's Disease remote monitoring system based on WSN
Maciucă, Popescu, Strutu, Stamatescu {2013} [81]	On-body Off-body	blood pressure, Heart Rate, blood oxygen saturation, heart rate, body temperature, Body Positioning, Pressure, Humidity, Carbon Dioxide, Explosive Gas, Ambient Light, Ambient Temperature	ZigBee, Femtocell	Proposes a smart hybrid sensor network for indoor monitoring using a multilayer femtocell
Gonzalez, Villegas, Ramirez, Sanchez, Dominguez {2014} [82]	On-Body	Heart Rate, Body Temperature	Wi-Fi, Smartphone, PC	Presents a system for remote monitoring based on mobile augmented reality (MAR) and WSN
Augustyniak {2013} [83]	On-body Off-body	Heart Rate, Body Positioning, Motion, sound	WiFi, GPRS, PDA, Smartphone	Proposes general rules of design of complex universal systems for health and behavior-based surveillance of human
ElSayed, Alosebai, Salaheldin, El Gayar, ElHelw {2010} [84]	On-body Off-body	Body Positioning, Motion	Unknown, PC	Applies real-time target extraction and a skeletonization procedure to quantify the motion of moving target
Lv, Xia, Wu, Yao, Chen {2010} [85]	On-body	Heart Rate, Blood Pressure, Body Positioning, Location (GPS)	Bluetooth, GSM, GPRS, Smartphone, PDA	This system contains some functions to assist elderly such as regular reminder, quick alarm, medical guidance
Megalingam, Unnikrishnan, Radhakrishnan, Jacob {2012} [86]	On-body	Heart Rate (PPG), body Temperature, Body Positioning	Bluetooth, GSM, Smartphone	Monitors the posture of the patient in the bed (tilt monitoring) in order to help to reduce the cases of bedsore in bedridden elders

Shimokawara, Kaneko, Yamaguchi, Mizukawa, Matsuhira {2013} [87]	On-body	Body Positioning	ZigBee, Sink Node	Focused on recognizing advanced motions (11 motions) by using 3D acceleration sensor
Baek, Kim, Bashir, Pyun {2013} [88]	On-body	Body Positioning (Accelerometer & Gyroscope)	ZigBee, Sink Node	A new fall detection system is proposed by using one sensor node which can be worn as a necklace
Jit, Maniyeri, Gopalakrishnan, Louis, Eugene, Palit, Siang, Seng, Xiaorong {2010} [89]	On-body	Body Positioning	Bluetooth, 3G, GPRS, WiFi, Smartphone (Windows based), PDA	Monitors the activity of individuals at night, through the use of simple wearable accelerometers
Steffen, Bleser, Weber, Stricker, Fradet, Marin {2011} [90]	On-body	Heart Rate, Body Positioning	Bluetooth, GSM, Smartphone	This work presents a methodology for an appropriate monitoring of strength training. The results are translated into appropriate feedback to the user
Tolkiehn, Atallah, Lo, Yang {2011} [91]	On-body	Body Positioning, Body Pressure	Unknown, PC	Uses a waist-worn sensor for reliable fall detection and the determination of the direction of a fall
Doukas, Maglogiannis {2011} [92]	On-body	Heart Rate, Body Temperature, Blood Oxygen, Body Positioning,	Bluetooth, GSM, Smartphone (Android-Based)	Textile platform based on open hardware and software, collects on-body data and stores them wirelessly on an open Cloud infrastructure
Megalingam, Radhakrishnan, Jacob, Unnikrishnan, Sudhakaran {2011} [93]	On-body	Heart Rate, Blood Oxygen, Body Temperature, Body Pressure	Bluetooth, GSM, PC	The proposed system is a compact device which has various wearable sensors all attached inside a glove which continuously monitors vital parameters of the elderly person
Singh, Muthukumarasamy {2011} [94]	On-body	Heart Rate, Blood Pressure, Temperature, Blood Oxygen	Proprietary, GSM, Smartphone	Shows how a group key can be securely established between the different sensors within a BAN
Sardini, Serpelloni, Ometto {2011} [95]	On-body	ECG, Heart Rate, Respiration Rate, Body Positioning	Bluetooth, GSM, PC, Smartphone	Proposes a system consists of a T-shirt sensorized to continuously record and analyzed human parameters during work activities at home
Lo, Valenzuela, Leung {2012} [96]	On-body	Atmospheric Air Pressure	ZigBee, PC	Presents a new approach to identifying and verifying the location of wearable wireless sensor nodes placed on a body by inferring differences in altitudes using atmospheric air pressure sensors
Wang, Wang, Shi {2012} [97]	On-body	Heart Rate, Blood Oxygen, Body Temperature, Respiration Rate, Pulse Rate	ZigBee, GPRS, Smartphone (Android-Based)	Proposes a new approach to monitor patients based on distributed WBAN

Goutham, Iyer, Rajiv {2010} [98]	On-body	ECG, Body Temperature	Bluetooth, GSM, PDA, Smartphone	Designs a periodic data management system to manage wireless interface of sensor units with the patient database
Rotariu, Costin, Andruseac, Ciobotariu, Adochiei {2011} [99]	On-body	Heart Rate, Respiratory Rhythm, Oxygen Saturation, Blood Pressure, Body Temperature	ZigBee, WiFi, GSM,GPRS, PDA	Proposes a system suitable for continuous long-time monitoring, as a part of a diagnostic procedure or can achieve medical assistance of a chronic condition
Apostu, Hagi, Pasca {2011} [100]	On-body	ECG	ZigBee, PC	Presents the development of a system for wireless ECG monitoring
Megalingam, Vineeth, Krishnan, Akhil, Jacob {2011} [101]	On-body	ECG, Blood Pressure, Heart Beat Rate, Body Temperature	Proprietary, GPRS, GSM, PC	Proposes a network based Wireless patient monitoring system, which can monitor multiple patients in hospital to measure various physical parameters
Manzoor, Javaid, Bibi, Khan, Tahir {2012} [102]	On-body	Unknown	ZigBee, GSM, PDA	Evaluates different types of interferences and disturbances such as ISI, MUI and noise through different techniques such as MUD receivers, DES-CMA and link adaptation
Wang, Gui, Liu, Chen, Jin {2013} [103]	On-body	Heart Rate, Blood Pressure, Respiration Rate, Oxygen Saturation	Bluetooth, GSM, Smartphone (Android-Based)	Reports preliminary study results that characterize the performance, energy, and complexity attributes of both mobile and cloud-based solutions for medical monitoring

729 6.1. Survey Results

730 Among the articles that are included in Table 14, seven articles consider off-body (ambient) sensors
731 along with on-body sensors [75] [76] [78] [79] [81] [83] [84]. In many of these articles, a data fusion
732 technique is used to integrate multiple data sources into meaningful information. The other 28 articles
733 investigate only on-body sensors [69-74] [77] [80] [82] [85-103].

734 Moreover, half of the articles employ mobile devices such as smart phones or PDAs as base stations.
735 Therefore, classic Bluetooth is considered as the main wireless communication technology in the
736 majority of the included articles.

737 On the other hand, 14 studies used ZigBee as the main wireless communication technology [73] [75]
738 [77-81] [87] [88] [96] [97] [99] [100] [102]. Therefore, ZigBee is considered the second most popular
739 technology among the included articles. However, surprisingly, in none of the included studies is
740 BLE used, which is likely to be explained because BLE is a relatively recent technology.

741 Many of these articles such as [70] [74] [78] [88] [91] focus on fall detection systems based on various
742 sensor types and different techniques. Therefore, fall detection is considered the most widely
743 researched topics in elderly monitoring systems. A number of articles such as [72] [74] [83] [89]
744 concentrate on Activities of Daily Living (ADL) of patients and elderly people. A few of these articles
745 also investigate specific chronic conditions such as anxiety [71], chronic obstructive pulmonary and
746 chronic kidney [76] and Parkinson's disease [69] [80].

747 The majority of the residential environment eHealthcare systems collected in this section used one of
748 the popular wireless technologies such as Bluetooth or ZigBee. All systems reviewed in Table 14
749 appear to have a high power requirement especially when compared to home-based eHealthcare
750 system requirements. When power is of little concern, the choice of wireless is less critical and
751 designers usually choose ones they are familiar with, easy to implement or in certain scenarios ones
752 which fit with existing infrastructure (WiFi, GSM, etc). A home environment eHealthcare system has
753 tight restrictions on power consumption, which therefore rule out many protocols including WiFi
754 and classic Bluetooth, even ZigBee.

755 Recent home-based patient monitoring systems as summarized in Table 14 focus on health
756 monitoring. It is apparent that most solutions are concerned with monitoring short-term acute
757 conditions where high power consumption – hence regular charging – can be justified, others may
758 be more suitable for longer operation with a single charge. There is however a distinct lack of
759 application of alternative wireless technologies or even Bluetooth Low Energy. This may be due to
760 aforementioned need to interface with infrastructure or other devices.

761 7. Conclusion

762 As a true home-based patient monitoring system is to transparently monitor individuals in home
763 environment over extended periods of time, sensor power requirements are of utmost importance.
764 Hence it is imperative that the employed wireless technologies have minimal power consumption. If
765 the application and choice of communication technology allow, energy harvesting based operation
766 has the potential to power the devices indefinitely. It is expected that in the years following this
767 survey a large body of research will accumulate with systems utilizing devices that require no specific
768 attention from those they monitor (i.e. charging). These systems would therefore allow devices to be
769 worn in everyday clothing and be operating continuously.

770 References

- 771 1. Office of National Statistics (2013). Statistical Bulletin National Population Projections, 2012-based
772 Statistical Bulletin. [Online]. Available: http://www.ons.gov.uk/ons/dcp171778_334975.pdf
- 773 2. U. C. B. P. I. Office. (2009, July). Unprecedented Global Aging Examined in New Census
774 Bureau Report Commissioned by the National Institute on Aging. U.S. Census Bureau.
775 Washington, DC. [Online]. Available:
776 https://www.census.gov/newsroom/releases/archives/aging_population/cb09-108.html
- 777 3. C. Wei and L. Jinju. (2009, Sept.). Future Population Trends in China: 2005-2050. Centre of
778 Policy Studies/IMPACT Centre, Victoria University. A u s t r a l i a . [Online]. Available:
779 <http://www.copsmodels.com/ftp/workpaper/g-191.pdf>
- 780 4. Department of Economic and Social Affairs Population Division, "World Population Prospects: The
781 2012 Revision. Methodology of the United Nations Population Estimates and Projections," UN., NY,
782 Rep. *ESA/P/WP.235*, 2004.
- 783 5. A. Alwan. (2011). Global status report on non-communicable diseases 2010. World Health
784 Org. Geneva, Switzerland. [Online]. Available:
785 http://www.who.int/nmh/publications/ncd_report_full_en.pdf
- 786 6. M. Chen, S. Gonzalez, A. Vasilakos, H. Cao, and V.C.M. Leung, "Body Area Networks: A Survey,"
787 *Mobile Networks and Applications*, vol. 16, no. 2, pp. 171-193, August 2010.
- 788 7. B. Latre, B. Braem, I. Moerman, C. Blondia, P. Demeester, "A Survey on Wireless Body Area
789 Networks," *ACM Journal of Wireless Networks*, vol. 17, no. 1, pp. 1-18, January. 2011.

- 790 8. University of Bristol, "SPHERE," 2015. [Online]. Available: <http://www.irc-sphere.ac.uk/about>.
791 [Accessed: 10-Mar-2015].
- 792 9. K. Iniewski, *VLSI Circuits for Biomedical Applications*. Norwood: Artech House, 2008
- 793 10. M. Ghamari, B. M. Heravi, U. Roedig, B. Honary, and C. A. Pickering, "Improving transmission
794 reliability of low-power medium access control protocols using average diversity combining," *IET*
795 *Wireless Sensor Systems*, vol. 2, no. 4, pp. 377–384, Dec. 2012.
- 796 11. M. Ghamari, B. Momahed Heravi, U. Roedig, and B. Honary, "Reliability comparison of
797 transmit/receive diversity and error control coding in low-power medium access control protocols,"
798 *IET Networks*, vol. 3, no. 4, pp. 284–292, Nov. 2014.
- 799 12. M. Ghamari, B. Janko, R. S. Sherratt, and W. Harwin, "An Energy-Efficient Hybrid System for
800 Wireless Body Area Network Applications," in *15th Ann. Post-Graduate Symposium on Convergence of*
801 *Telecomm., Networking and Broadcasting.*, Liverpool, UK, 2014
- 802 13. W. R. Dieter, S. Datta, W.K. Kai, "Power Reduction by Varying Sampling Rate," in *IEEE International*
803 *Symposium on Low Power Electronics and Design.*, San Diego, USA, 2005
- 804 14. A. Krause, M. Ihmig, E. Rankin, D. Leong, S. Gupta, D. Siewiorek, A. Smailagic, M. Deisher, U.
805 Sengupta, "Trading off Prediction Accuracy and Power Consumption for Context-Aware Wearable
806 Computing," in *9th IEEE International Symposium on Wearable Computers.*, Osaka, Japan, 2005
- 807 15. Smart Data Sampling and Data Reconstruction, by A. Cuyt, W.S. Lee. (2014, July 10).
808 US20140195200A1. Available: <http://www.google.com/patents/EP2745404A1?cl=en>
- 809 16. Y. Zhao, Y. Hao, A. Alomainy and C. Parini, "UWB On-Body Radio Channel Modeling using Ray
810 Theory and Subband FDTD Method," *IEEE Transaction on Microwave Theory and Techniques*, vol. 54,
811 no. 4, pp. 1827-1835, June. 2006.
- 812 17. L. Liu, R. D'Errico, L. Ouvry, P. De Doncker and C. Oestges, "Dynamic Channel Modeling at 2.4 GHz
813 for On-Body Area Networks," *Journal of Advances in Electronics and Telecommunications*, vol. 2, no. 4.
814 pp. 18-27, December. 2011.
- 815 18. S. V. Roy, F. Quitin, L. F. Liu, C. Oestges, F. Horlin, J. M. Dricot and P. De Doncker, "Dynamic
816 Channel Modeling for Multi-Sensor Body Area Networks," *IEEE Transaction on Antennas and*
817 *Propagation*, vol. 61, no. 4, pp. 2200-2208, December. 2012
- 818 19. C. Chakraborty, B. Gupta, S. K. Ghosh, and C. Engineering, "A Review on Telemedicine-Based
819 WBAN Framework for Patient Monitoring," vol. 19, no. 8, pp. 619–626, 2013.
- 820 20. A. Arya, N. Bilandi, "A Review : Wireless Body Area Networks for Health Care," *International Journal*
821 *of Innovative Research in Computer and Communication Engineering*, vol. 2, no. 4, pp. 3800–3806, 2014.
- 822 21. Bluetooth SIG (2015). Bluetooth Low Energy. [Online]. Available:
823 <http://www.bluetooth.com/Pages/low-energy-tech-info.aspx>
- 824 22. *IEEE Standard for Local and Metropolitan Area Networks — Part 15.4: Low-Rate Wireless Personal Area*
825 *Networks (LR-WPANs)*, IEEE Standard 802.15.4, 2011.
- 826 23. ZigBee Alliance (2015). [Online]. Available: <http://www.zigbee.org/>
- 827 24. ZigBee. (2009, March). ZigBee Wireless Sensor Applications for Health, Wellness and Fitness. ZigBee
828 Alliance, Davis, CA. [Online]. Available:
829 <http://www.science.smith.edu/~jcardell/Courses/EGR328/Readings/Zigbee&HealthCare.pdf>
- 830 25. *IEEE Standard for Health Informatics - Personal Health Device Communication Part 00103: Overview*, IEEE
831 Standard 11073-00103, 2012.


- 832 26. ZigBee. (2012, December). New ZigBee PRO Feature : Green Power. ZigBee Alliance, Davis, CA.
833 [Online]. Available: <https://docs.zigbee.org/zigbee-docs/dcn/12/docs-12-0646-01-0mwg-new-zigbee->
834 [pro-feature-green-power.pdf](https://docs.zigbee.org/zigbee-docs/dcn/12/docs-12-0646-01-0mwg-new-zigbee-pro-feature-green-power.pdf)
- 835 27. K. S. Kwak, S. Ullah, and N. Ullah, "An Overview of IEEE 802.15.6 Standard," in *International*
836 *Symposium on Applied Science in Biomedical and Communication Technologies.*, Rome, Italy, 2010
- 837 28. Bluetooth (2015). [Online]. Available: <http://www.bluetooth.com/Pages/Bluetooth-Home.aspx>
- 838 29. Bluetooth Development Portal (2015). [Online]. Available:
839 <https://developer.bluetooth.org/TechnologyOverview/Pages/HDP.aspx>
- 840 30. ANT+ (2015). [Online]. Available: <http://www.thisisant.com/>
- 841 31. RuBee (2015). [Online]. Available: <http://www.rubee.com/>
- 842 32. *IEEE Standard for Long Wavelength Wireless Network Protocol*, IEEE Standard 1902.1, 2009.
- 843 33. X. Yu, X. Xia, and X. Chen, "Design and application of RuBee-based telemedicine data acquisition
844 system," in *10th IEEE International Conference on Computer and Information Science.*, Sanya, China, 2011
- 845 34. M. Zareei, A. Zarei, R. Budiarto, and M. A. Omar, "A Comparative Study of Short Range Wireless
846 Sensor Network on High Density Networks," *17th Asia-Pacific Conference on Communications.*, Sabah,
847 Malaysia, 2011
- 848 35. Toumaz Group (2015). [Online]. Available: <http://www.toumaz.com/>
- 849 36. I. F. Akyildiz, W. Su, Y. Sankarasubramaniam, and E. Cayirci, "A Survey on Sensor Networks," *IEEE*
850 *Communications Magazine*, vol. 40, no. 8, pp. 102-114, November. 2002.
- 851 37. Microsemi (2015) [Online]. Available: <http://www.microsemi.com/>
- 852 38. Zarlink Semiconductor. (2009). "ZL70101 Medical Implantable RF Transceiver" [Online]. Available:
853 <http://ulp.zarlink.com/zarlink/zweb-zl70101-datasheet-dec09.pdf>
- 854 39. Insteon (2015) [Online]. Available: <http://www.insteon.com/>
- 855 40. S. Adibi, "Link technologies and BlackBerry mobile Health (mHealth) solutions: A review," *IEEE*
856 *Transactions on Information Technology in Biomedicine*, vol. 16, no. 4, pp. 586-597, June. 2012.
- 857 41. Z-Wave (2015). [Online]. Available: <http://www.z-wave.com>
- 858 42. Sigma Designs (2015). [Online]. Available: <http://www.sigmadesigns.com/>
- 859 43. Z-Wave Alliance (2015). [Online]. Available: <http://z-wavealliance.org/>
- 860 44. C. Gomez and J. Paradells, "Wireless home automation networks: A survey of architectures and
861 technologies," *IEEE Communications Magazine*, vol. 48, no. 6, pp. 92-101, June. 2010.
- 862 45. Elster (2015). "Wavenis Technology" [Online]. Available: <http://www.elstermetering.com/en/wavenis->
863 [technology](http://www.elstermetering.com/en/wavenis-technology)
- 864 46. FitLinxx (2015). "BodyLAN Wireless Protocol" [Online]. Available: <http://www.fitlinxx.net/bodylan->
865 [wireless-protocol.htm](http://www.fitlinxx.net/bodylan-wireless-protocol.htm)
- 866 47. DASH7 Alliance (2015). [Online]. Available: <http://www.dash7-alliance.org/>
- 867 48. One-Net (2015). [Online]. Available: <http://www.one-net.info/>
- 868 49. EnOcean (2015). [Online]. Available: <https://www.enocean.com/en/home/>
- 869 50. M. Seyedi, B. Kibret, D. T. H. Lai, and M. Faulkner, "A survey on intrabody communications for body
870 area network applications," *IEEE Transactions on Biomedical Engineering*, vol. 60, no. 8, pp. 2067-2079,
871 July. 2013.
- 872 51. M. S. Wegmueller, M. Oberle, N. Felber, N. Kuster, and W. Fichtner, "Signal transmission by galvanic
873 coupling through the human body," *IEEE Transactions on Instrumentation and Measuremen.*, vol. 59,
874 no. 4, pp. 963-969, March. 2009.

- 875 52. L. Galluccio, T. Melodia, S. Palazzo and G. E. Santagati, "Challenges and Implications of using
876 Ultrasonic Communications in Intra-body Area Networks," in *9th International Conference on Wireless
877 On-Demand Network Systems and Services*, Courmayeur, Italy, 2012
- 878 53. M. Ghamari, H. Arora, R. S. Sherratt, and W. Harwin, "Comparison of Low-Power Wireless
879 Communication Technologies for Wearable Health-Monitoring Applications," in *2th IEEE
880 International Conference on Computer, Communications and Control Technology.*, Kuching, Malaysia, 2015
- 881 54. Z. Spasojevic, J. Burns, "Performance Comparison of Frequency Hopping and Direct Sequence Spread
882 Spectrum Systems in the 2.4 GHz Range," in *11th IEEE International Symposium on Personal Indoor and
883 Mobile Radio Communications.*, London, UK, 2000
- 884 55. Nordic. (2001, January). "nRF903 430MHz-950MHz Single Chip RF Transceiver" [Online]. Available:
885 <http://www.go-gddq.com/download/NRF/NRF903.pdf>
- 886 56. P. Sikka, P. Corke, and L. Overs, "Wireless sensor devices for animal tracking and control," in *29th
887 IEEE International Conference on Local Computer Networks.*, Washington, DC, 2004
- 888 57. W. Z. Khan, Y. Xiang, M. Y. Aalsalem, and Q. Arshad, "Mobile Phone Sensing Systems: A Survey,"
889 *IEEE Communaction Survey & Tutorials*, vol. 15, no. 1, pp. 402–427, April. 2013.
- 890 58. Y. Zhang, L. Sun, H. Song, and X. Cao, "Ubiquitous WSN for Healthcare: Recent Advances and
891 Future Prospects," *IEEE Journal of Internet of Things*, vol. 1, no. 4, pp. 311-318, June. 2014.
- 892 59. M. Kumar, A. Veeraraghavan, and A. Sabharwal, "DistancePPG: Robust non-contact vital signs
893 monitoring using a camera," *Journal of Biomedical Optic Express*, vol. 6, no. 5, pp. 1565-1588, April.
894 2015.
- 895 60. T. Hao, G. Xing, and G. Zhou, "iSleep : Unobtrusive Sleep Quality Monitoring using Smartphones," in
896 *11th ACM Conference on Embedded Networked Sensor Systems.*, NY, USA, 2013
- 897 61. S. Kwon, H. Kim, and K. S. Park, "Validation of heart rate extraction using video imaging on a built-in
898 camera system of a smartphone," in *IEEE International Conference of Engineering in Medicine and Biology
899 Society.*, San Diego, CA, 2012
- 900 62. T. Hao, G. Xing, and G. Zhou, "Unobtrusive Sleep Monitoring using Smartphones," in *7th International
901 Conference on Pervasive Computing Technologies for Healthcare.*, Venice, Italy, 2013
- 902 63. M. Frost, G. Marcu, R. Hansen, K. Szaanto, and J. E. Bardram, "The MONARCA self-assessment
903 system: Persuasive personal monitoring for bipolar patients," in *5th International Conference on
904 Pervasive Computing Technologies for Healthcare.*, Dublin, Ireland, 2011
- 905 64. J. Lee. (2015, March). Biometrics combined with big data will impact the healthcare industry [Online].
906 Available: [http://www.biometricupdate.com/201503/biometrics-combined-with-big-data-will-impact-
907 the-healthcare-industry](http://www.biometricupdate.com/201503/biometrics-combined-with-big-data-will-impact-the-healthcare-industry)
- 908 65. D. Ryan, D. Price, S. D. Musgrave, S. Malhotra, a. J. Lee, D. Ayansina, a. Sheikh, L. Tarassenko, C.
909 Pagliari, and H. Pinnock, "Clinical and cost effectiveness of mobile phone supported self monitoring
910 of asthma: multicentre randomised controlled trial," *BMJ Journal*, vol. 344, pp. e1756, March. 2012.
- 911 66. J. Escarrabill (2013, July). Telemonitoring in patients with chronic respiratory diseases : lights and
912 shadows [Online]. Available: [file:///C:/Users/nw906304/Downloads/31_erg-0003-2012%20\(6\).pdf](file:///C:/Users/nw906304/Downloads/31_erg-0003-2012%20(6).pdf)
- 913 67. P. Zanaboni and R. Wootton, "Adoption of telemedicine: from pilot stage to routine delivery," *BMC
914 Medical Informatics& Decision Making*, vol. 12, no. 1, January. 2012.
- 915 68. A. Parmar (2014, April). 5 Areas of mHealth Growth In The Future [Online]. Available:
916 <http://www.mddionline.com/article/5-areas-mhealth-growth-future>

- 917 69. M. Dorfman, E. Gazit, A. Mirelman, J. M. Hausdorff, and G. T. R. Oster, "A Wearable Assistant for
918 Gait Training for Parkinson's Disease with Freezing of Gait in Out-of-the-Lab Environments," *ACM*
919 *Transaction on Interactive Intelligent Systems*, vol. 5, no. 1, March. 2015.
- 920 70. A. Taylor, F. E. Park, L. Bernard, M. C. Health, S. C. Partnership, S. Hospital, D. Road, H. Pizey, C.
921 Whittet, S. Davies, D. Hammond, J. Edge, C. C. Care, and S. Road, "BodyGuard : A Case Study of
922 Telecare," in *33th ACM Conference Extended Abstracts on Human Factors in Computing Systems.*, NY,
923 USA, 2015
- 924 71. D. Miranda, M. Calderón, and J. Favela, "Anxiety detection using wearable monitoring," in *ACM*
925 *Conference on Human Computer Interaction.*, NY, USA, 2014
- 926 72. E. Kantoch, P. Augustyniak, M. Markiewicz, and D. Prusak, "Monitoring activities of daily living
927 based on wearable wireless body sensor network," in *IEEE International Conference on Engineering in*
928 *Medicine and Biology Society.*, Chicago, USA, 2014
- 929 73. P. M. Papazoglou, "Towards a Low Cost Open Architecture Wearable Sensor Network for Health
930 Care Applications," in *7th International Conference on Pervasive Technologies Related to Assistive*
931 *Environments.*, NY, USA, 2014
- 932 74. O. Ojetola, E. Gaura, and J. Brusey, "Data Set for Fall Events and Daily Activities from Inertial
933 Sensors," in *6th ACM Conference on Multimedia Systems.*, NY, USA, 2015
- 934 75. H. Yan, H. Huo, Y. Xu, and M. Gidlund, "Wireless sensor network based E-health system ??
935 implementation and experimental results," *IEEE Transaction on Consumer Electronics*, vol. 56, no. 4,
936 pp. 2288–2295, November. 2010.
- 937 76. R. Farre, a. Papadopoulos, G. Munaro, and R. Rosso, "An Open, Ubiquitous and Adaptive Chronic
938 Disease Management Platform for Chronic Respiratory and Renal Diseases (CHRONIOUS)," in
939 *International Conference on eHealth, Telemedicine and Social Medicine.*, Cancun, Mexico, 2009
- 940 77. P. Vanveerdeghem, P. Van Torre, C. Stevens, J. Knockaert, and H. Rogier, "Synchronous Wearable
941 Wireless Body Sensor Network Composed of Autonomous Textile Nodes," *Journal of Sensors*, vol. 14,
942 pp. 18583–18610, October. 2014.
- 943 78. C. N. Doukas and I. Maglogiannis, "Emergency fall incidents detection in assisted living
944 environments utilizing motion, sound, and visual perceptual components," *IEEE Transactions on*
945 *Information Technology in Biomedicine*, vol. 15, no. 2, pp. 277–289, November. 2011.
- 946 79. G. Lamprinakos, E. Kosmatos, D. Kaklamani, and I. S. Venieris, "An integrated architecture for
947 remote healthcare monitoring," in *14th Panhellenic Conference on Informatics.*, Tripoli, Libya, 2010
- 948 80. J. Cancela, M. Pastorino, M. T. Arredondo, K. S. Nikita, F. Villagra, and M. a Pastor, "Feasibility Study
949 of a Wearable System Based on a Wireless Body Area Network for Gait Assessment in Parkinson's
950 Disease Patients," *Journal of Sensors*, vol. 14, no. 3, pp. 4618–4633, March. 2014.
- 951 81. A. Maciuca, D. Popescu, M. Strutu, and G. Stamatescu, "Wireless sensor network based on multilevel
952 femtocells for home monitoring," in *IEEE International Conference on Intelligent Data Acquisition*
953 *Advanced Computing Systems.*, Berlin, Germany, 2013
- 954 82. F. González, O. Villegas, D. Ramírez, V. Sánchez, and H. Domínguez, "Smart Multi-Level Tool for
955 Remote Patient Monitoring Based on a Wireless Sensor Network and Mobile Augmented Reality,"
956 *Journal of Sensors*, vol. 14, no. 9, pp. 17212–17234, September. 2014.
- 957 83. P. Augustyniak, "Adaptive architecture for assisted living systems," in *6th International Conference on*
958 *Human System Interaction.*, Sopot, Poland, 2013

- 959 84. M. El Sayed, a. Alsebai, a. Salaheldin, N. El Gayar, and M. ElHelw, "Body and visual sensor fusion for
960 motion analysis in Ubiquitous healthcare systems," in *International Conference on Body Sensor*
961 *Networks.*, Singapore, 2010
- 962 85. Z. Lv, F. Xia, G. Wu, L. Yao, and Z. Chen, "iCare: A mobile health monitoring system for the elderly,"
963 in *IEEE International Conference on Green Computing and Communications*, Hangzhou, China, 2010
- 964 86. R. K. Megalingam, D. K. M. Unnikrishnan, V. Radhakrishnan, and D. C. Jacob, "HOPE: An electronic
965 gadget for home-bound patients and elders," in *IEEE India Conference.*, Kochi, India, 2012
- 966 87. E. Shimokawara, T. Kaneko, T. Yamaguchi, M. Mizukawa, and N. Matsuhira, "Estimation of Basic
967 Activities of Daily Living Using ZigBee 3D Accelerometer Sensor Network," in *IEEE International*
968 *Conference on Biometrics and Kansei.*, Tokyo, Japan, 2013
- 969 88. F. Bashir, "Real life applicable fall detection system based on wireless body area network," in *IEEE*
970 *Conference on Consumer Communications and networking.*, Las Vegas, USA, 2013
- 971 89. B. Jit, J. Maniyeri, K. Gopalakrishnan, S. Louis, P. J. Eugene, H. N. Palit, F. Y. Siang, L. L. Seng, X. Li,
972 and Ieee, "Processing of wearable sensor data on the cloud - a step towards scaling of continuous
973 monitoring of health and well-being," in *International Conference of Engineering in Medicine and Biology*
974 *Society.*, Buenos Aires, Argentina, 2010
- 975 90. D. Steffen, G. Bleser, M. Weber, D. Stricker, L. Fradet, and F. Marin, "A Personalized Exercise Trainer
976 for Elderly," in *5th International Conference on Pervasive Computing Technologies for Healthcare.*, Dublin,
977 Ireland, 2011
- 978 91. M. Tolkiehn, L. Atallah, B. Lo, and G.-Z. Yang, "Direction sensitive fall detection using a triaxial
979 accelerometer and a barometric pressure sensor," in *International Conference of Engineering in Medicine*
980 *and Biology.*, Boston, USA, 2011
- 981 92. C. Doukas and I. Maglogiannis, "Managing Wearable Sensor Data through Cloud Computing," in
982 *IEEE International Conference on Cloud Computing Technology and Science.*, Athens, Greece, 2011
- 983 93. R. K. Megalingam, V. Radhakrishnan, D. C. Jacob, D. K. M. Unnikrishnan, and A. K. Sudhakaran,
984 "Assistive technology for elders: Wireless intelligent healthcare gadget," in *IEEE Conference on Global*
985 *Humanitarian Technology.*, Seattle, USA, 2011
- 986 94. K. Singh and V. Muthukkumarasamy, "Using physiological signals for authentication in a group key
987 agreement protocol," in *IEEE Conference on Computer Communications Workshop.*, Shanghai, China,
988 2011
- 989 95. E. Sardini, M. Serpelloni, M. Ometto, "Multi-parameters wireless shirt for Physiological Monitoring,"
990 in *IEEE International Workshop on Medical Measurements and Applications.*, Bari, Italy, 2011
- 991 96. G. Lo, S. Gonzalez-Valenzuela and V. C. M. Leung, "Automatic identification and placement
992 verification of wearable wireless sensor nodes using atmospheric air pressure distribution," in *IEEE*
993 *Conference on Consumer Communications and Networking.*, Las Vegas, USA, 2012
- 994 97. C. Wang, Q. Wang, and S. Shi, "A distributed wireless body area network for medical supervision,"
995 in *IEEE Conference on Instrumentation and Measurement Technology.*, Graz, Austria, 2012
- 996 98. A. A. Tahat, "Mobile messaging services-based personal electrocardiogram monitoring system,"
997 *International Journal of Telemedicine and Applications.*, vol. 2009, PP. 7, June. 2009.
- 998 99. C. Rotariu, H. Costin, G. Andruseac, R. Ciobotariu, and F. Adochiei, "An integrated system for
999 wireless monitoring of chronic patients and elderly people," in *15th International Conference on System*
1000 *Theory Control and Computing.*, Sinaia, Romania, 2011

- 1001 100. O. Apostu, B. Hagi, and S. Pasca, "Wireless ECG monitoring and alarm system using ZigBee," in 7th
1002 *International Symposium on Advanced Topics in Electrical Engineering.*, Bucharest, 2011
- 1003 101. R. K. Megalingam, R. Vineeth, M. U. D. Krishnan, K. S. Akhil, and D. C. Jacob, "Advancetid network
1004 based wireless, single PMS for multiple-patient monitoring," in 13th *International Conference on*
1005 *Advanced Communication Technology.*, Seoul, Korea, 2011
- 1006 102. B. Manzoor, N. Javaid, a Bibi, Z. a Khan, M. Tahir, and Ieee, "Noise Filtering, Channel Modeling and
1007 Energy Utilization in Wireless Body Area Networks," in 3th *International Symposium on Advances in*
1008 *Embedded Systems and Applications.*, Liverpool, UK, 2012
- 1009 103. X. Wang, Q. Gui, B. Liu, Y. Chen, Z. Jin, and Ieee, "Leveraging Mobile Cloud for Telemedicine: A
1010 Performance Study in Medical Monitoring," in 39th *Bioengineering Conference.*, NY, USA, 2013



© 2016 by the authors; licensee MDPI, Basel, Switzerland. This article is an open access article distributed under the terms and conditions of the Creative Commons by Attribution (CC-BY) license (<http://creativecommons.org/licenses/by/4.0/>).